

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111220\
 Data File : FG007338.D
 Signal(s) : FID1A.ch
 Acq On : 12 Nov 2020 13:37
 Operator : DD\AJ
 Sample : L4714-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 13 01:06:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
 Quant Title :
 QLast Update : Tue Nov 03 02:04:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	2812229	22.859 ug/ml
Target Compounds			
4) N-TETRADECANE	8.233	151376	1.074 ug/ml
7) N-EICOSANE	12.644	200110	1.395 ug/ml
8) N-DOCOSANE	13.866	610898	4.351 ug/ml
10) N-TETRACOSANE	14.971	92850	0.665 ug/ml
12) N-OCTACOSANE	16.923	351809	2.649 ug/ml
13) N-TRIACONTANE	17.803	197435	1.535 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111220\
Data File : FG007338.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2020 13:37
Operator : DD\AJ
Sample : L4714-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 13 01:06:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

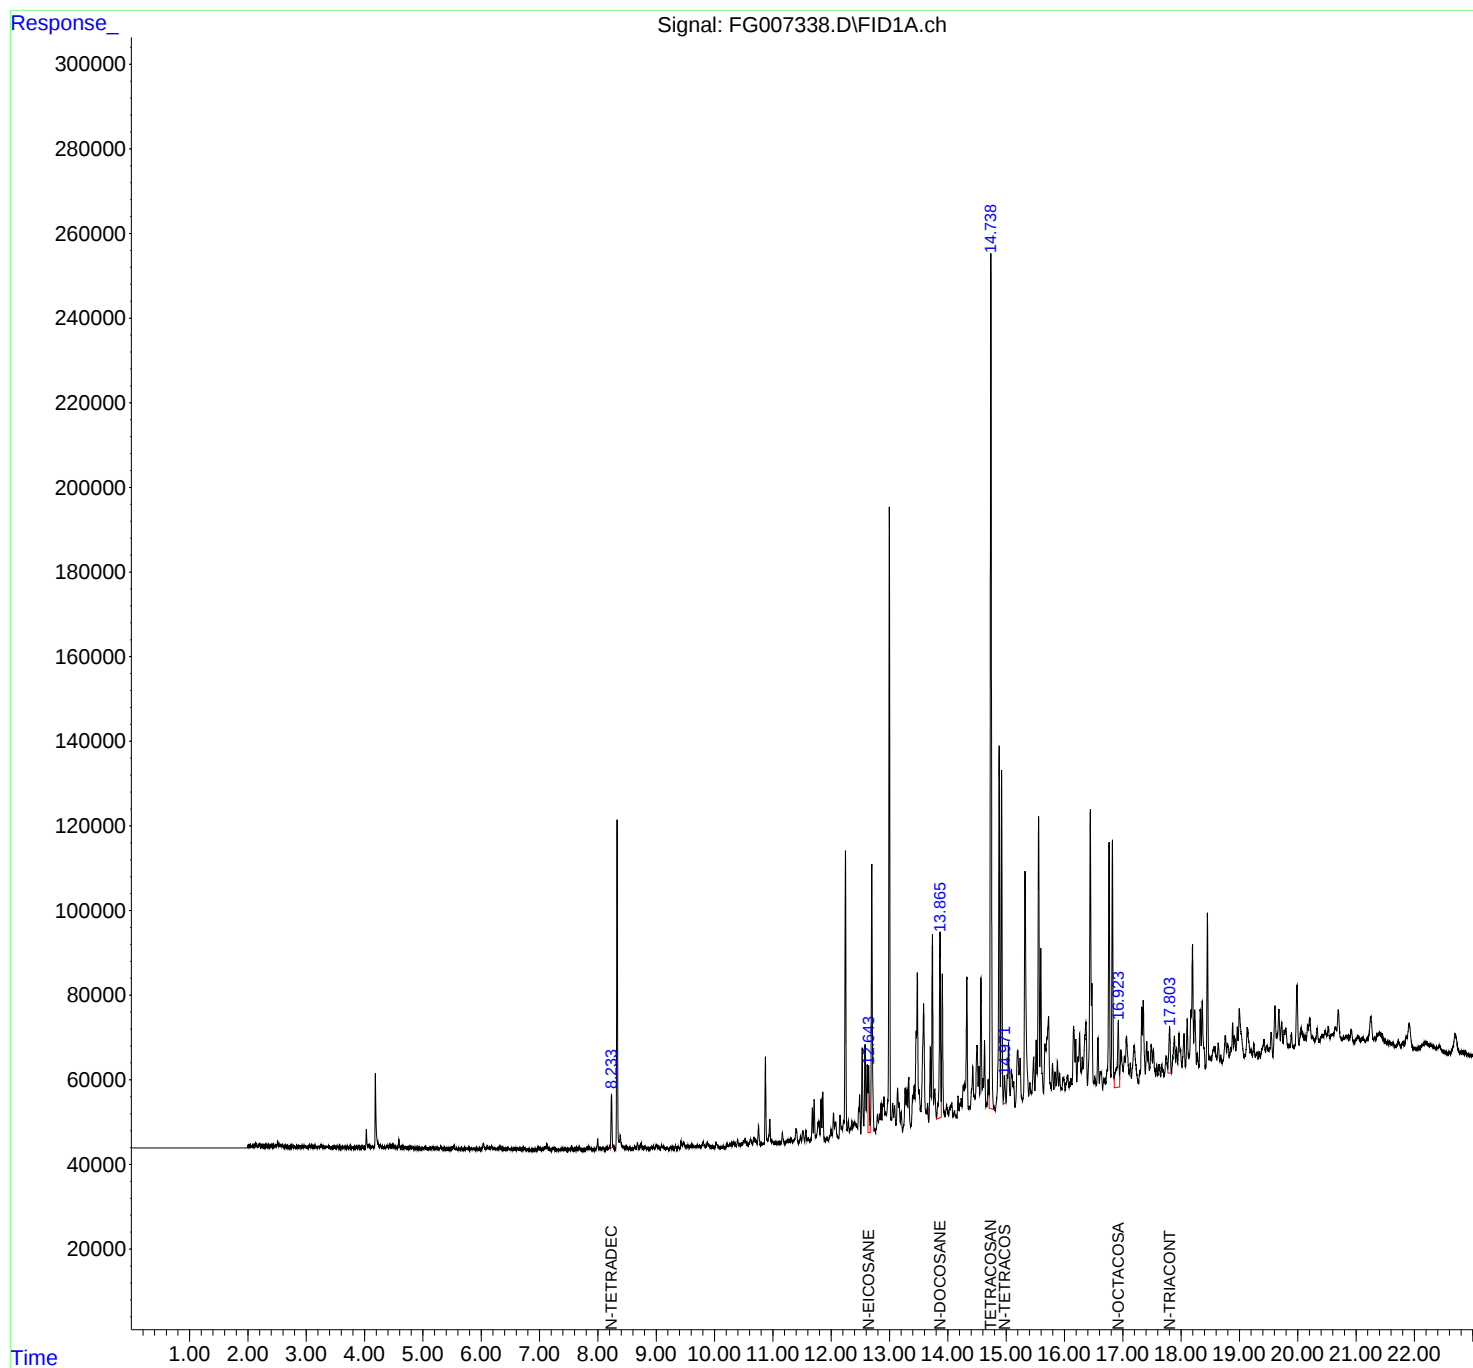


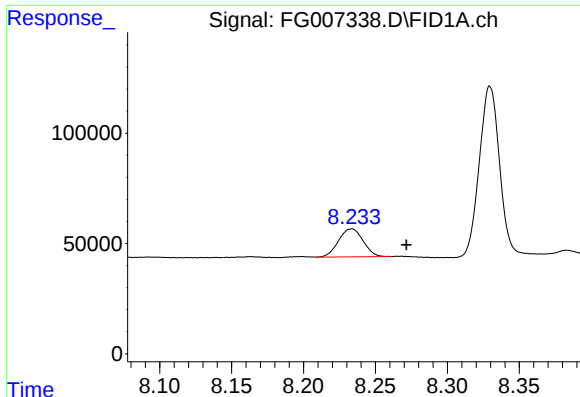

#4 N-TETRADECANE


R.T.: 8.233 min
Delta R.T.: -0.038 min
Response: 151376
Conc: 1.07 ug/ml

Instrument :
FID_G
ClientSampleId :

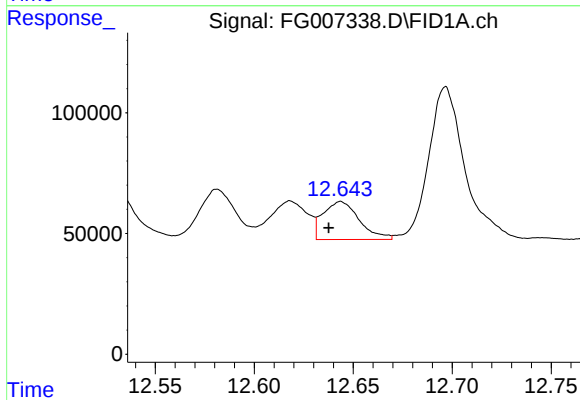


#7 N-EICOSANE

R.T.: 12.644 min
Delta R.T.: 0.006 min
Response: 200110
Conc: 1.40 ug/ml

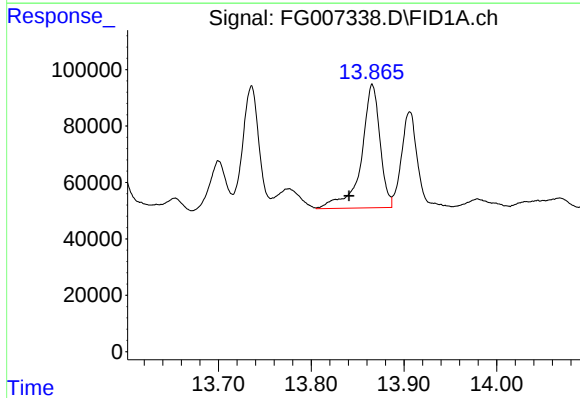


#8 N-DOCOSANE

R.T.: 13.866 min
Delta R.T.: 0.025 min
Response: 610898
Conc: 4.35 ug/ml

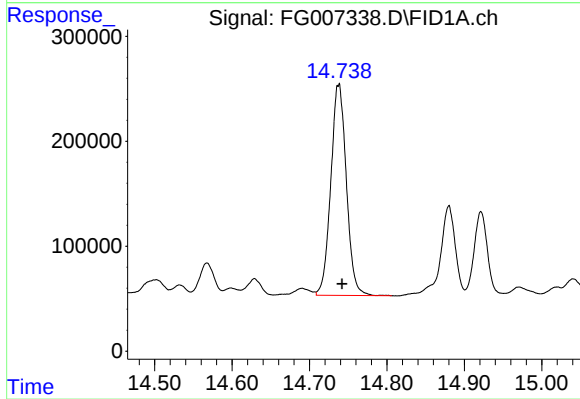

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.738 min
Delta R.T.: -0.005 min
Response: 2812229
Conc: 22.86 ug/ml

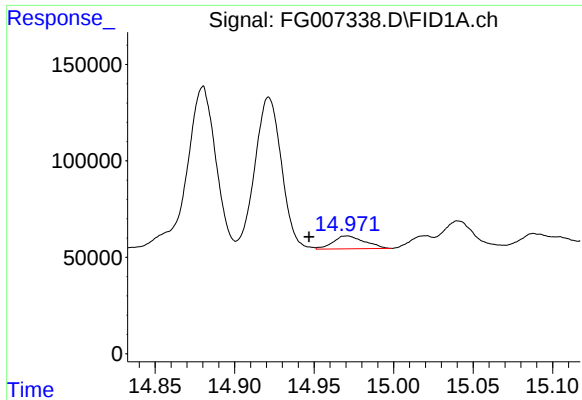

#10 N-TETRACOSANE


R.T.: 14.971 min
Delta R.T.: 0.024 min
Response: 92850
Conc: 0.67 ug/ml

Instrument :
FID_G
ClientSampleId :

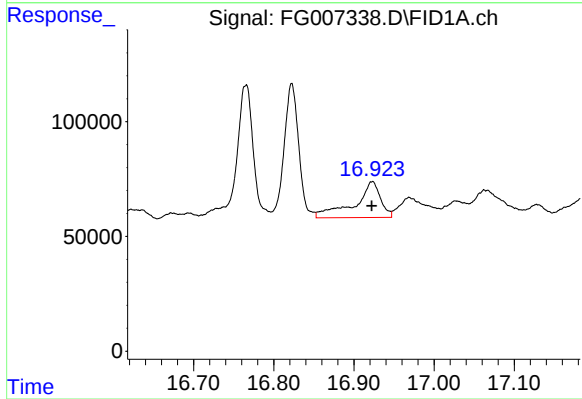

#12 N-OCTACOSANE

R.T.: 16.923 min
Delta R.T.: 0.000 min
Response: 351809
Conc: 2.65 ug/ml

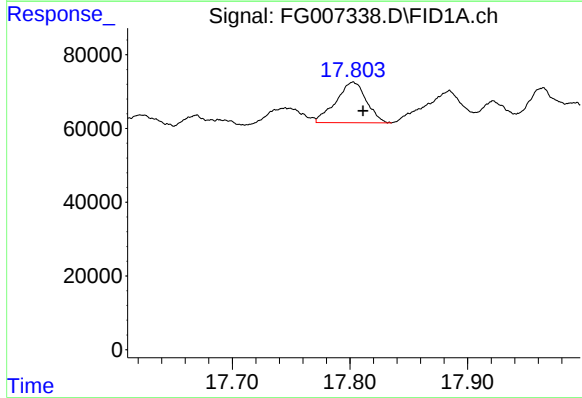

#13 N-TRIACONTANE

R.T.: 17.803 min
Delta R.T.: -0.008 min
Response: 197435
Conc: 1.54 ug/ml