

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111221\
Data File : FG009039.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2021 17:48
Operator : AJ\MA
Sample : M4661-04 50X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 21:44:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.733	386062	3.345 ug/ml
Target Compounds			
6) N-OCTADECANE	11.296	147746	1.078 ug/ml
7) N-EICOSANE	12.674	215198	1.573 ug/ml
10) N-TETRACOSANE	14.958	485115	3.673 ug/ml
11) N-HEXACOSANE	15.939	18310	0.144 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111221\
Data File : FG009039.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2021 17:48
Operator : AJ\MA
Sample : M4661-04 50X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 21:44:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

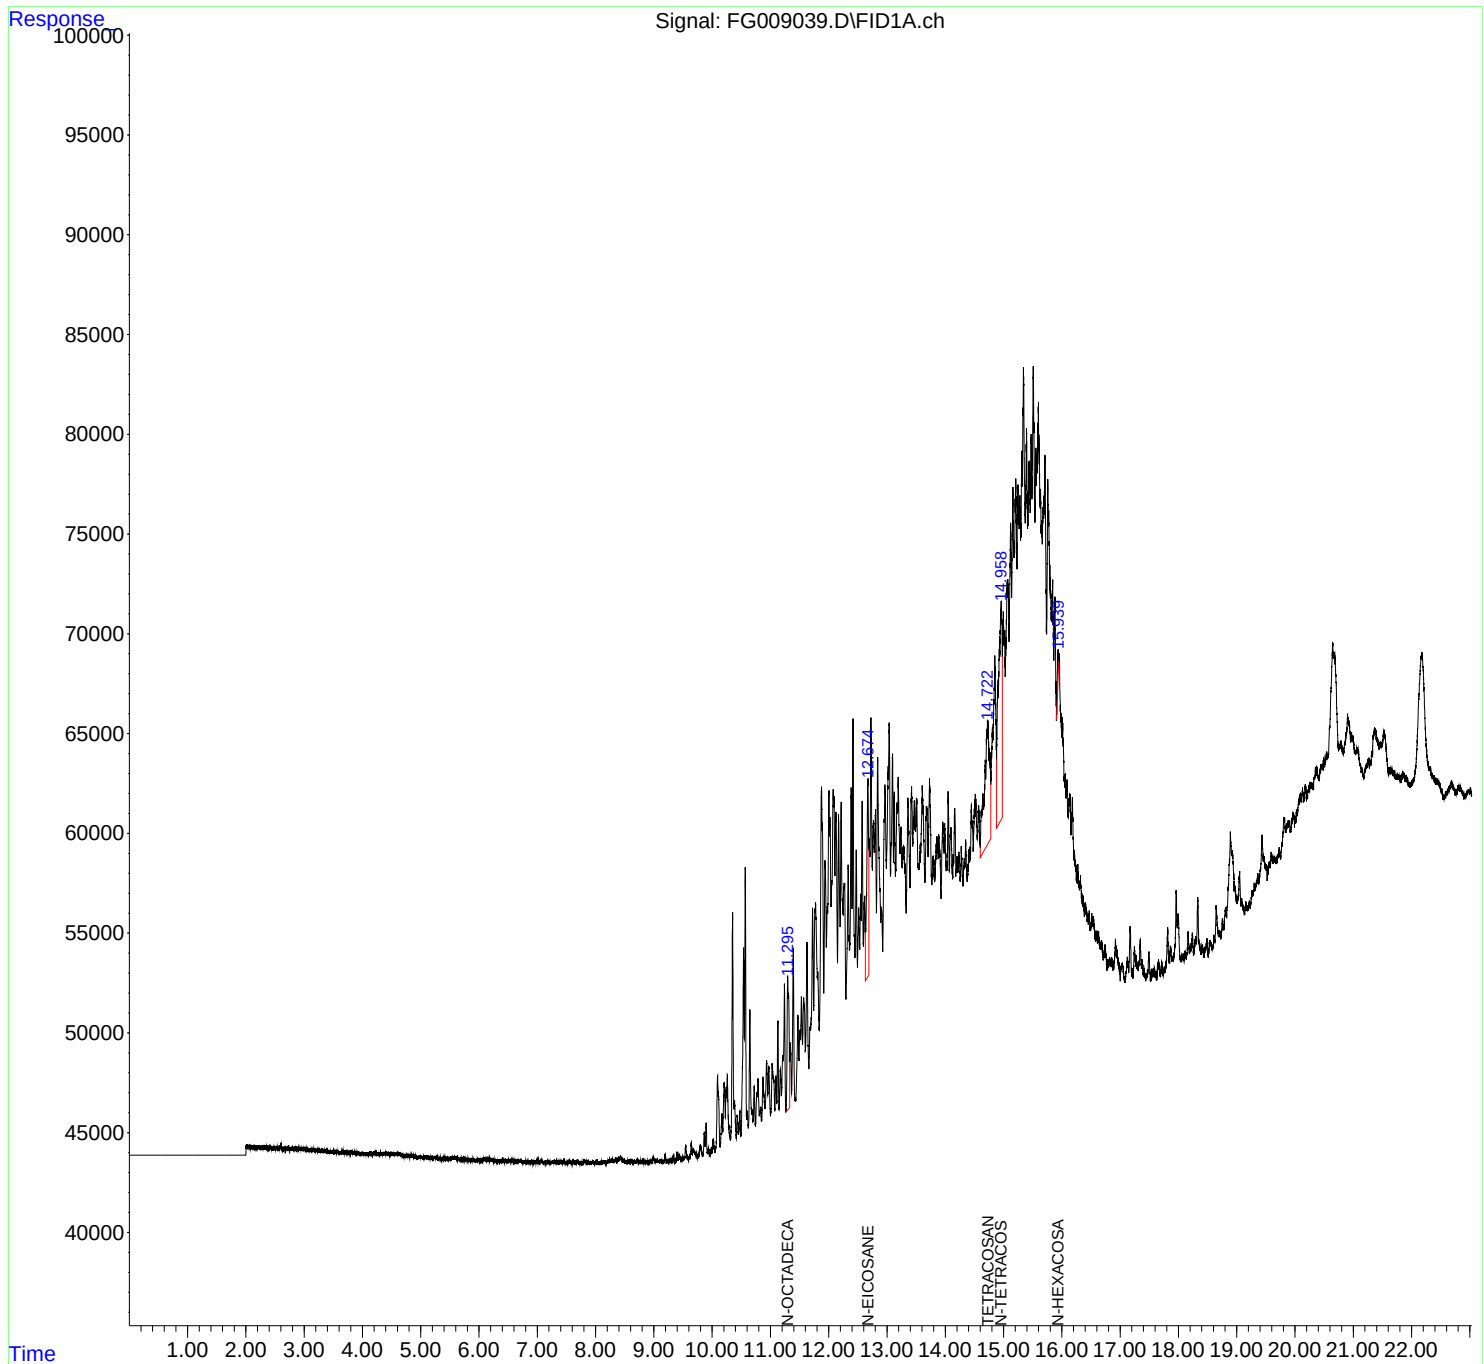


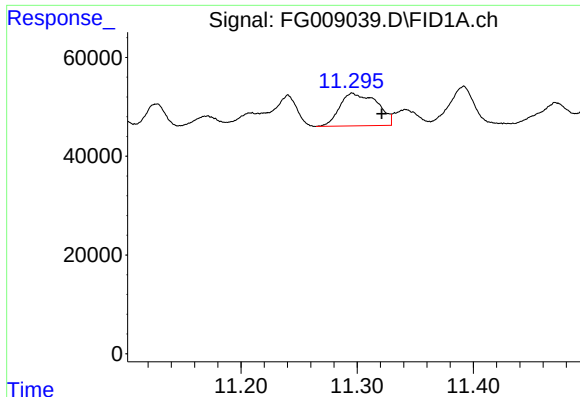

#6 N-OCTADECANE


R.T.: 11.296 min
Delta R.T.: -0.025 min
Response: 147746
Conc: 1.08 ug/ml

Instrument :
FID_G
ClientSampleId :

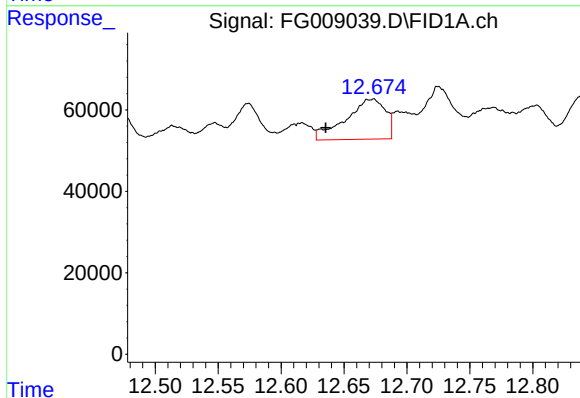


#7 N-EICOSANE

R.T.: 12.674 min
Delta R.T.: 0.038 min
Response: 215198
Conc: 1.57 ug/ml

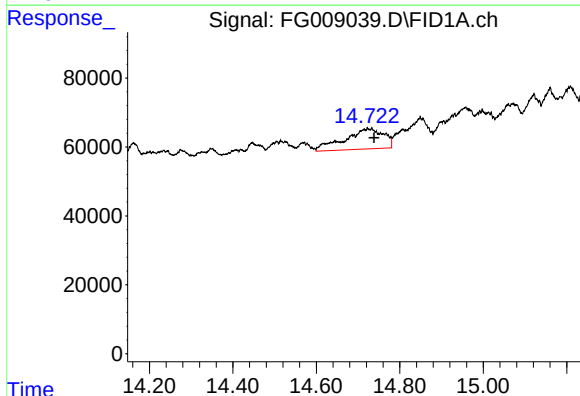


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.733 min
Delta R.T.: -0.005 min
Response: 386062
Conc: 3.34 ug/ml

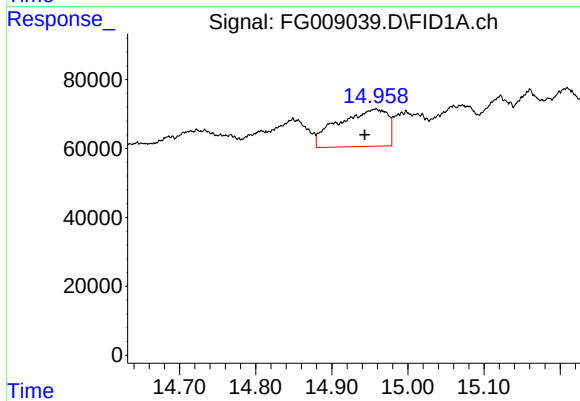

#10 N-TETRACOSANE

R.T.: 14.958 min
Delta R.T.: 0.015 min
Response: 485115
Conc: 3.67 ug/ml

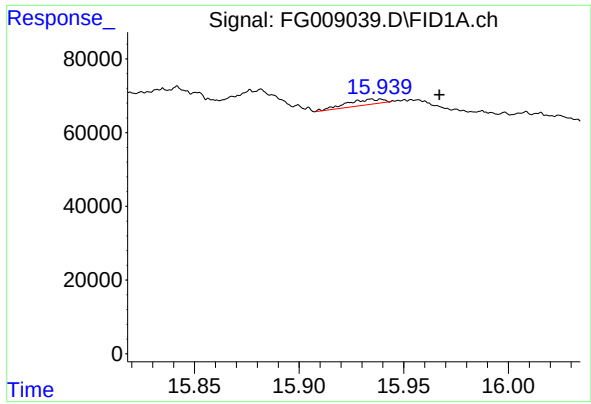

#11 N-HEXACOSANE

R.T.: 15.939 min
Delta R.T.: -0.028 min
Response: 18310
Conc: 0.14 ug/ml

Instrument :

FID_G

ClientSampleId :