

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111221\
Data File : FG009040.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2021 18:50
Operator : AJ\MA
Sample : PB140720BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 21:44:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.741	1786373	15.478 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.655	89874	0.826 ug/ml
15) N-TETRATRIACONTANE	19.439	55772	0.549 ug/ml
16) N-HEXATRIACONTANE	20.215	85551	0.907 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111221\
Data File : FG009040.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2021 18:50
Operator : AJ\MA
Sample : PB140720BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 12 21:44:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

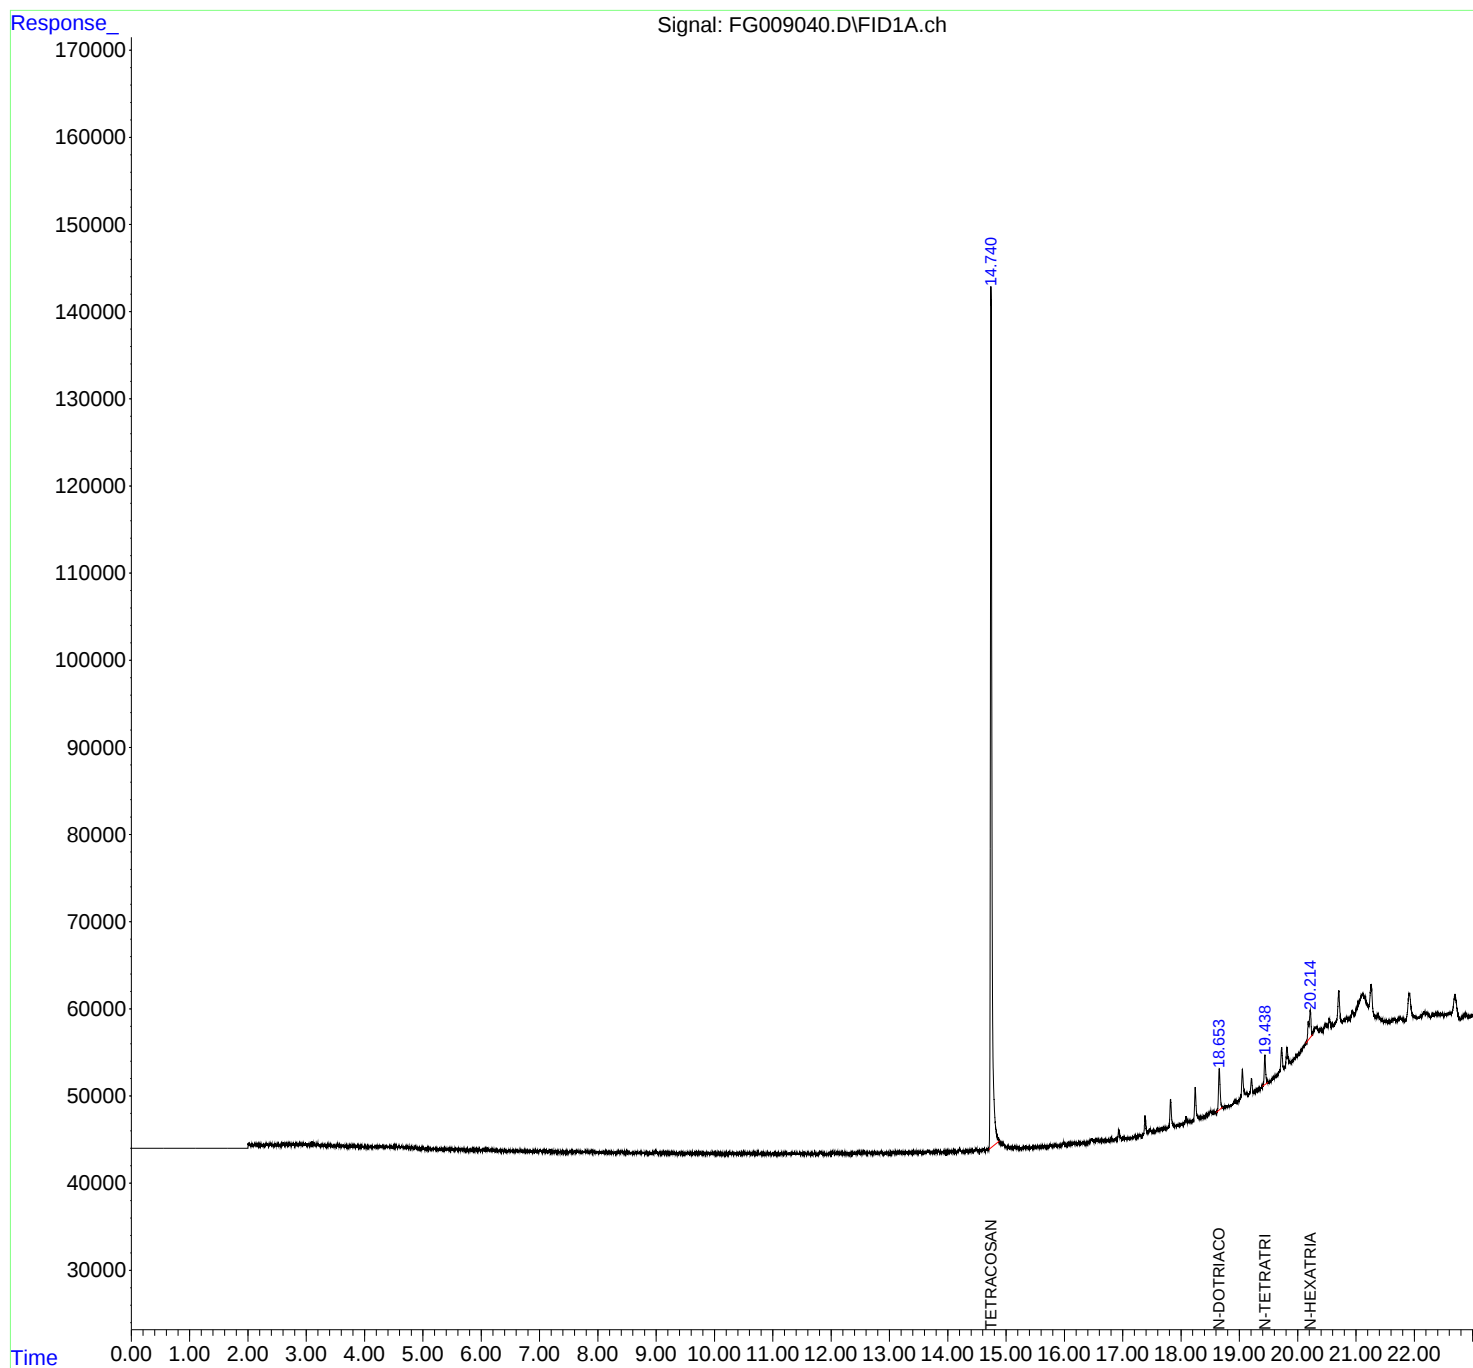


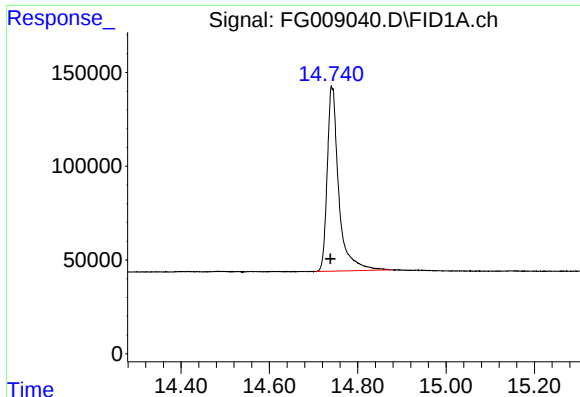

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.741 min
Delta R.T.: 0.002 min
Response: 1786373
Conc: 15.48 ug/ml

Instrument :
FID_G
ClientSampleId :

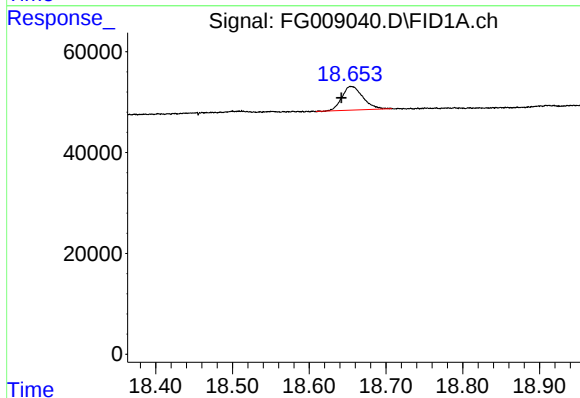


#14 N-DOTRIACONTANE

R.T.: 18.655 min
Delta R.T.: 0.013 min
Response: 89874
Conc: 0.83 ug/ml

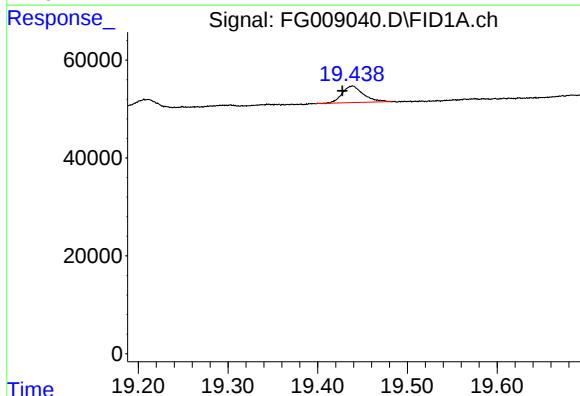

#15 N-TETRATRIACONTANE

R.T.: 19.439 min
Delta R.T.: 0.011 min
Response: 55772
Conc: 0.55 ug/ml

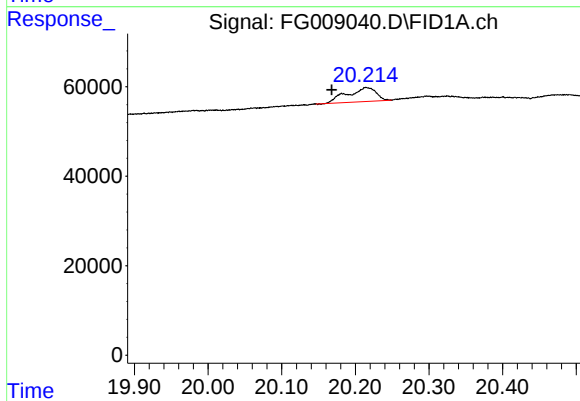

#16 N-HEXATRIACONTANE

R.T.: 20.215 min
Delta R.T.: 0.047 min
Response: 85551
Conc: 0.91 ug/ml