

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111221\
 Data File : FG009048.D
 Signal(s) : FID1A.ch
 Acq On : 12 Nov 2021 22:55
 Operator : AJ\MA
 Sample : M4644-06 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 13 00:36:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
 Quant Title :
 QLast Update : Tue Nov 02 01:56:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	139328	1.207 ug/ml
Target Compounds			
7) N-EICOSANE	12.617	1915	0.014 ug/ml
8) N-DOCOSANE	13.881	156624	1.170 ug/ml
10) N-TETRACOSANE	14.943	526385	3.985 ug/ml
12) N-OCTACOSANE	16.907	51541	0.419 ug/ml
13) N-TRIACONTANE	17.810	2594	0.022 ug/ml
14) N-DOTRIACONTANE	18.644	89409	0.821 ug/ml
15) N-TETRATRIACONTANE	19.434	45205	0.445 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111221\
Data File : FG009048.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2021 22:55
Operator : AJ\MA
Sample : M4644-06 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 13 00:36:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

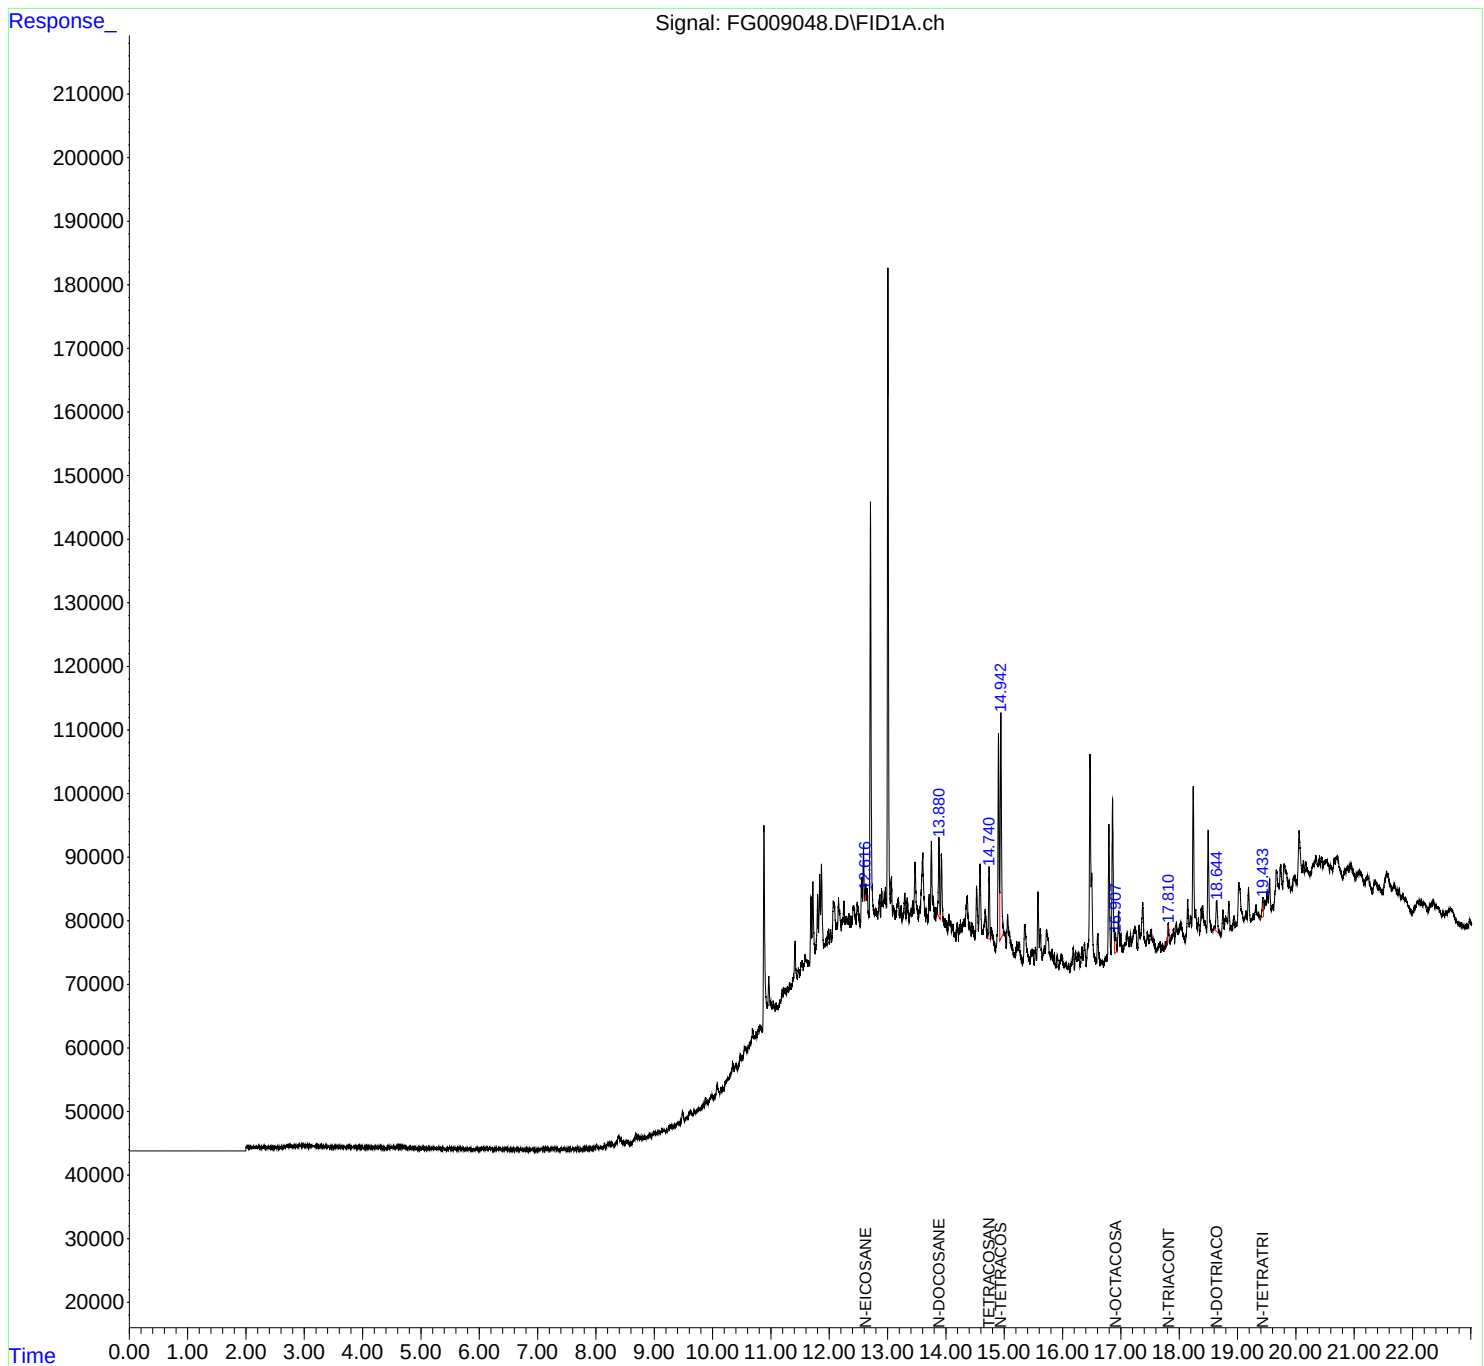


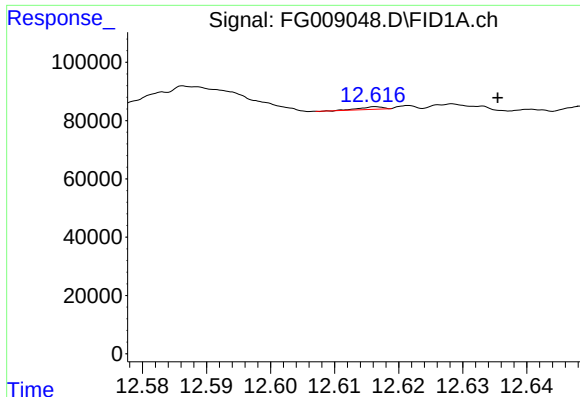

#7 N-EICOSANE


R.T.: 12.617 min
Delta R.T.: -0.019 min
Response: 1915
Conc: 0.01 ug/ml

Instrument :
FID_G
ClientSampleId :

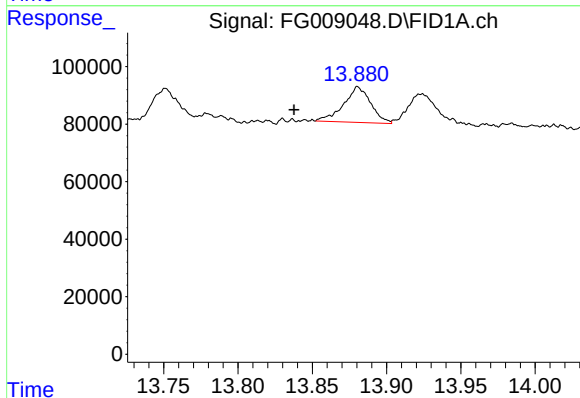


#8 N-DOCOSANE

R.T.: 13.881 min
Delta R.T.: 0.043 min
Response: 156624
Conc: 1.17 ug/ml

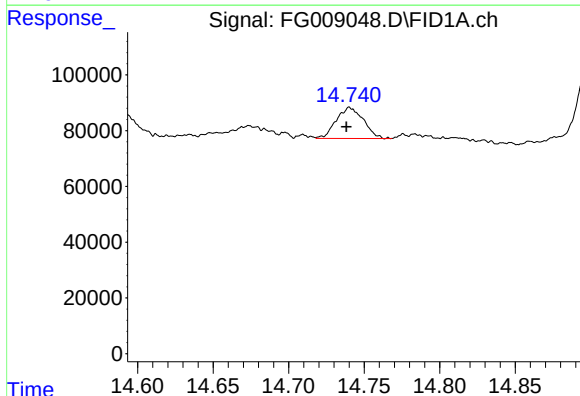


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.740 min
Delta R.T.: 0.002 min
Response: 139328
Conc: 1.21 ug/ml

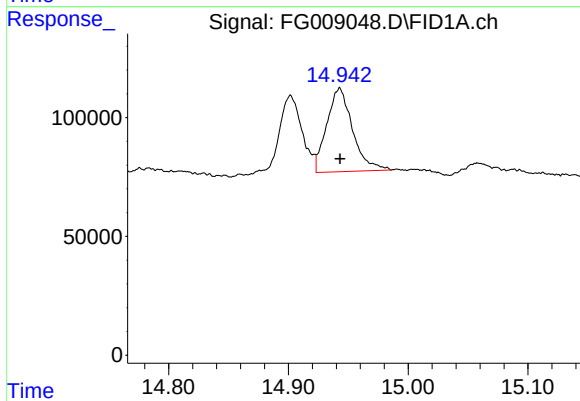

#10 N-TETRACOSANE


R.T.: 14.943 min
Delta R.T.: 0.000 min
Response: 526385
Conc: 3.99 ug/ml

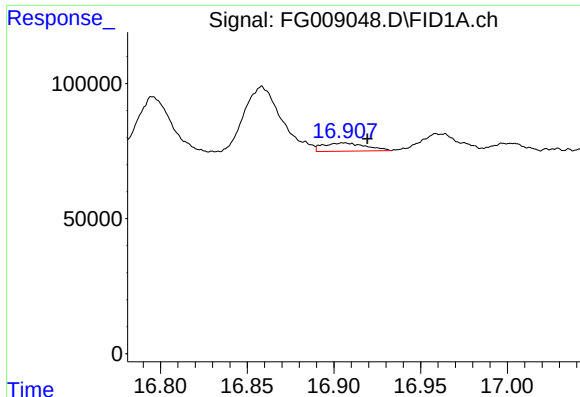

#12 N-OCTACOSANE


R.T.: 16.907 min
Delta R.T.: -0.013 min
Response: 51541
Conc: 0.42 ug/ml

Instrument :
FID_G
ClientSampleId :

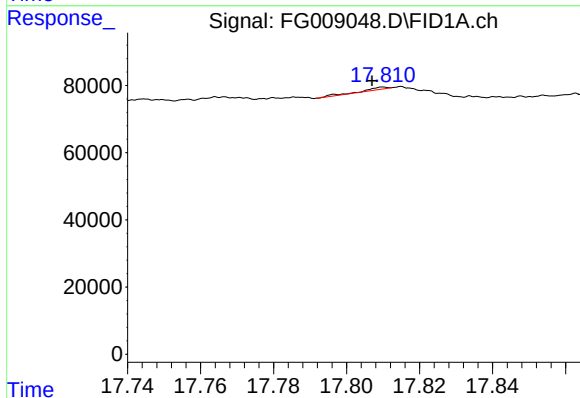


#13 N-TRIACONTANE

R.T.: 17.810 min
Delta R.T.: 0.003 min
Response: 2594
Conc: 0.02 ug/ml

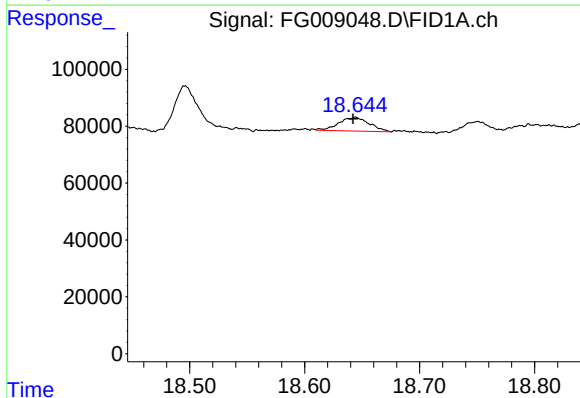

#14 N-DOTRIACONTANE

R.T.: 18.644 min
Delta R.T.: 0.002 min
Response: 89409
Conc: 0.82 ug/ml

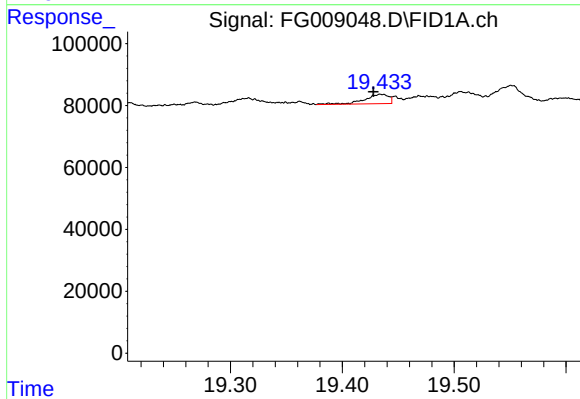

#15 N-TETRATRIACONTANE

R.T.: 19.434 min
Delta R.T.: 0.006 min
Response: 45205
Conc: 0.45 ug/ml