

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG111221\  
Data File : FG009057.D  
Signal(s) : FID1A.ch  
Acq On : 13 Nov 2021 03:29  
Operator : AJ\MA  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Nov 13 04:30:13 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG110121.M  
Quant Title :  
QLast Update : Tue Nov 02 01:56:13 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                          | R.T.    | Response | Conc Units  |
|-----------------------------|--------------------------|---------|----------|-------------|
| -----                       |                          |         |          |             |
| System Monitoring Compounds |                          |         |          |             |
| 9) S                        | TETRACOSANE-d50 (SURR... | 14.792f | 51438    | 0.446 ug/ml |
| Target Compounds            |                          |         |          |             |
| 14)                         | N-DOTRIACONTANE          | 18.657  | 24913    | 0.229 ug/ml |
| 15)                         | N-TETRATRIACONTANE       | 19.442  | 49166    | 0.484 ug/ml |
| 16)                         | N-HEXATRIACONTANE        | 20.177  | 72877    | 0.773 ug/ml |
| 17)                         | N-OCTATRIACONTANE        | 20.928  | 108506   | 1.226 ug/ml |
| -----                       |                          |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG111221\  
Data File : FG009057.D  
Signal(s) : FID1A.ch  
Acq On : 13 Nov 2021 03:29  
Operator : AJ\MA  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Nov 13 04:30:13 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG110121.M  
Quant Title :  
QLast Update : Tue Nov 02 01:56:13 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

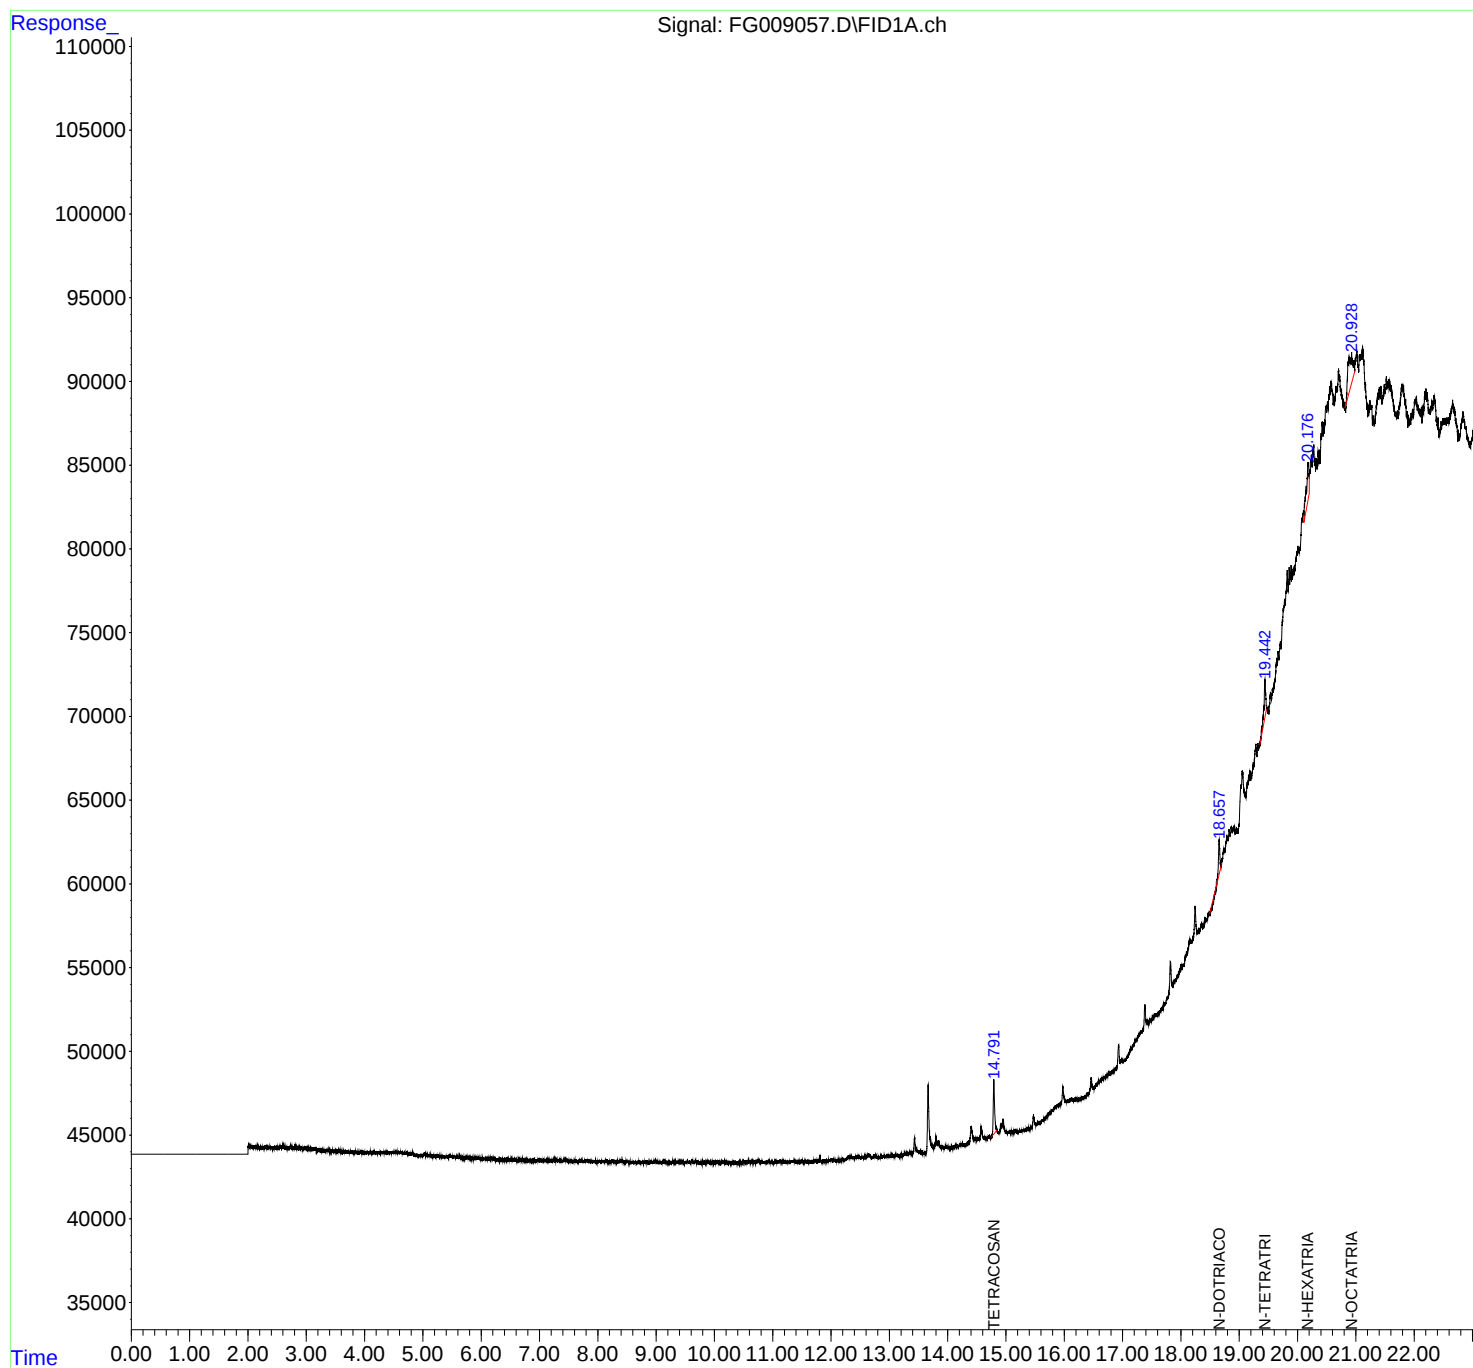


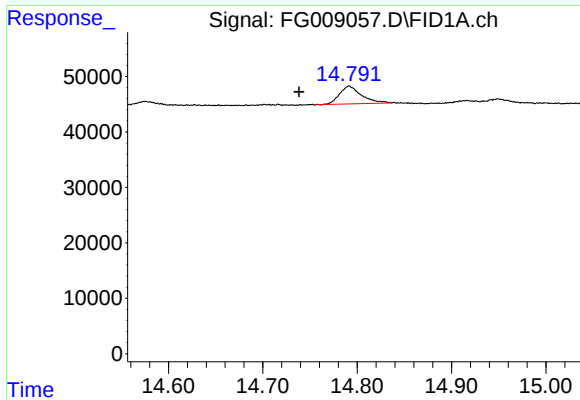

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.792 min  
Delta R.T.: 0.053 min  
Response: 51438  
Conc: 0.45 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

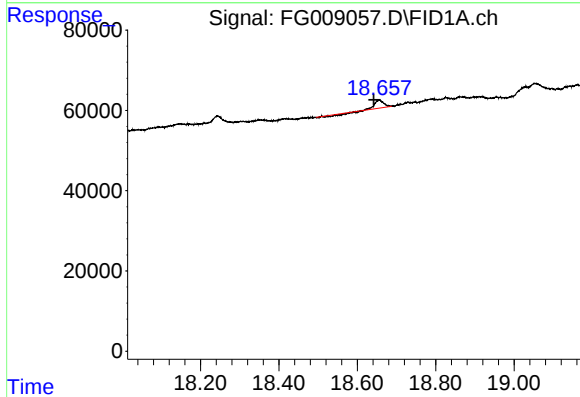


#14 N-DOTRIACONTANE

R.T.: 18.657 min  
Delta R.T.: 0.015 min  
Response: 24913  
Conc: 0.23 ug/ml

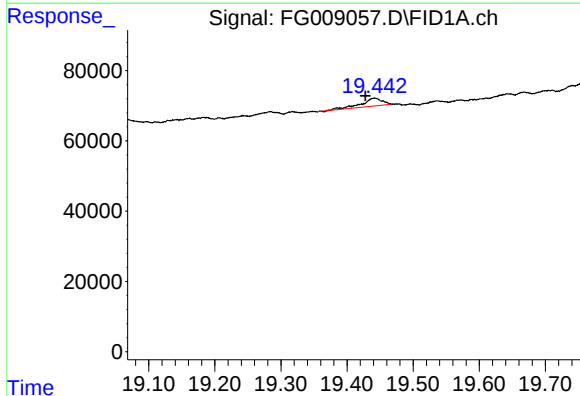


#15 N-TETRATRIACONTANE

R.T.: 19.442 min  
Delta R.T.: 0.015 min  
Response: 49166  
Conc: 0.48 ug/ml

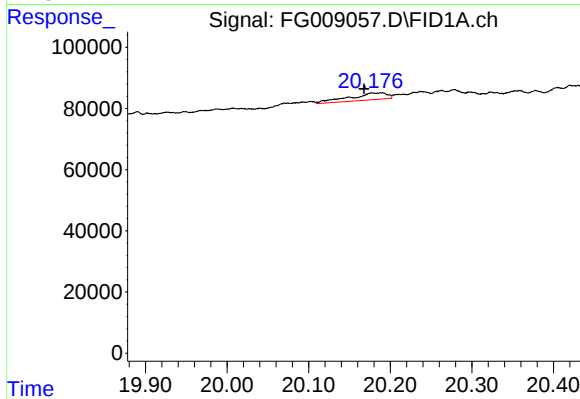

#16 N-HEXATRIACONTANE

R.T.: 20.177 min  
Delta R.T.: 0.009 min  
Response: 72877  
Conc: 0.77 ug/ml

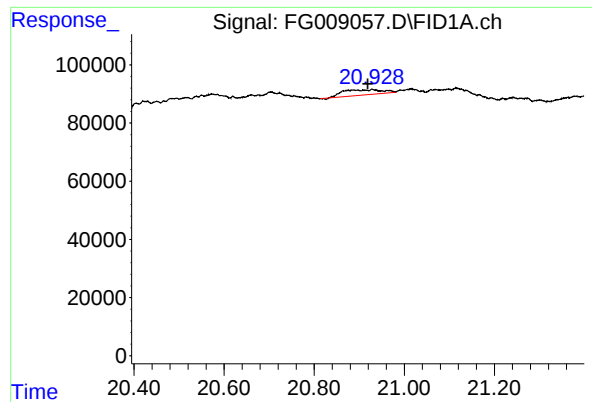

#17 N-OCTATRIACONTANE

R.T.: 20.928 min  
Delta R.T.: 0.009 min  
Response: 108506  
Conc: 1.23 ug/ml

Instrument :

FID\_G

ClientSampleId :