

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111221\
Data File : FG009034.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2021 15:14
Operator : AJ\MA
Sample : M4659-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
HB-1-(7.5-8)-11-11-21

Integration File: Sample.e
Quant Time: Nov 12 21:42:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.739	1961523	16.995 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111221\
Data File : FG009034.D
Signal(s) : FID1A.ch
Acq On : 12 Nov 2021 15:14
Operator : AJ\MA
Sample : M4659-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
HB-1-(7.5-8)-11-11-21

Integration File: Sample.e
Quant Time: Nov 12 21:42:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

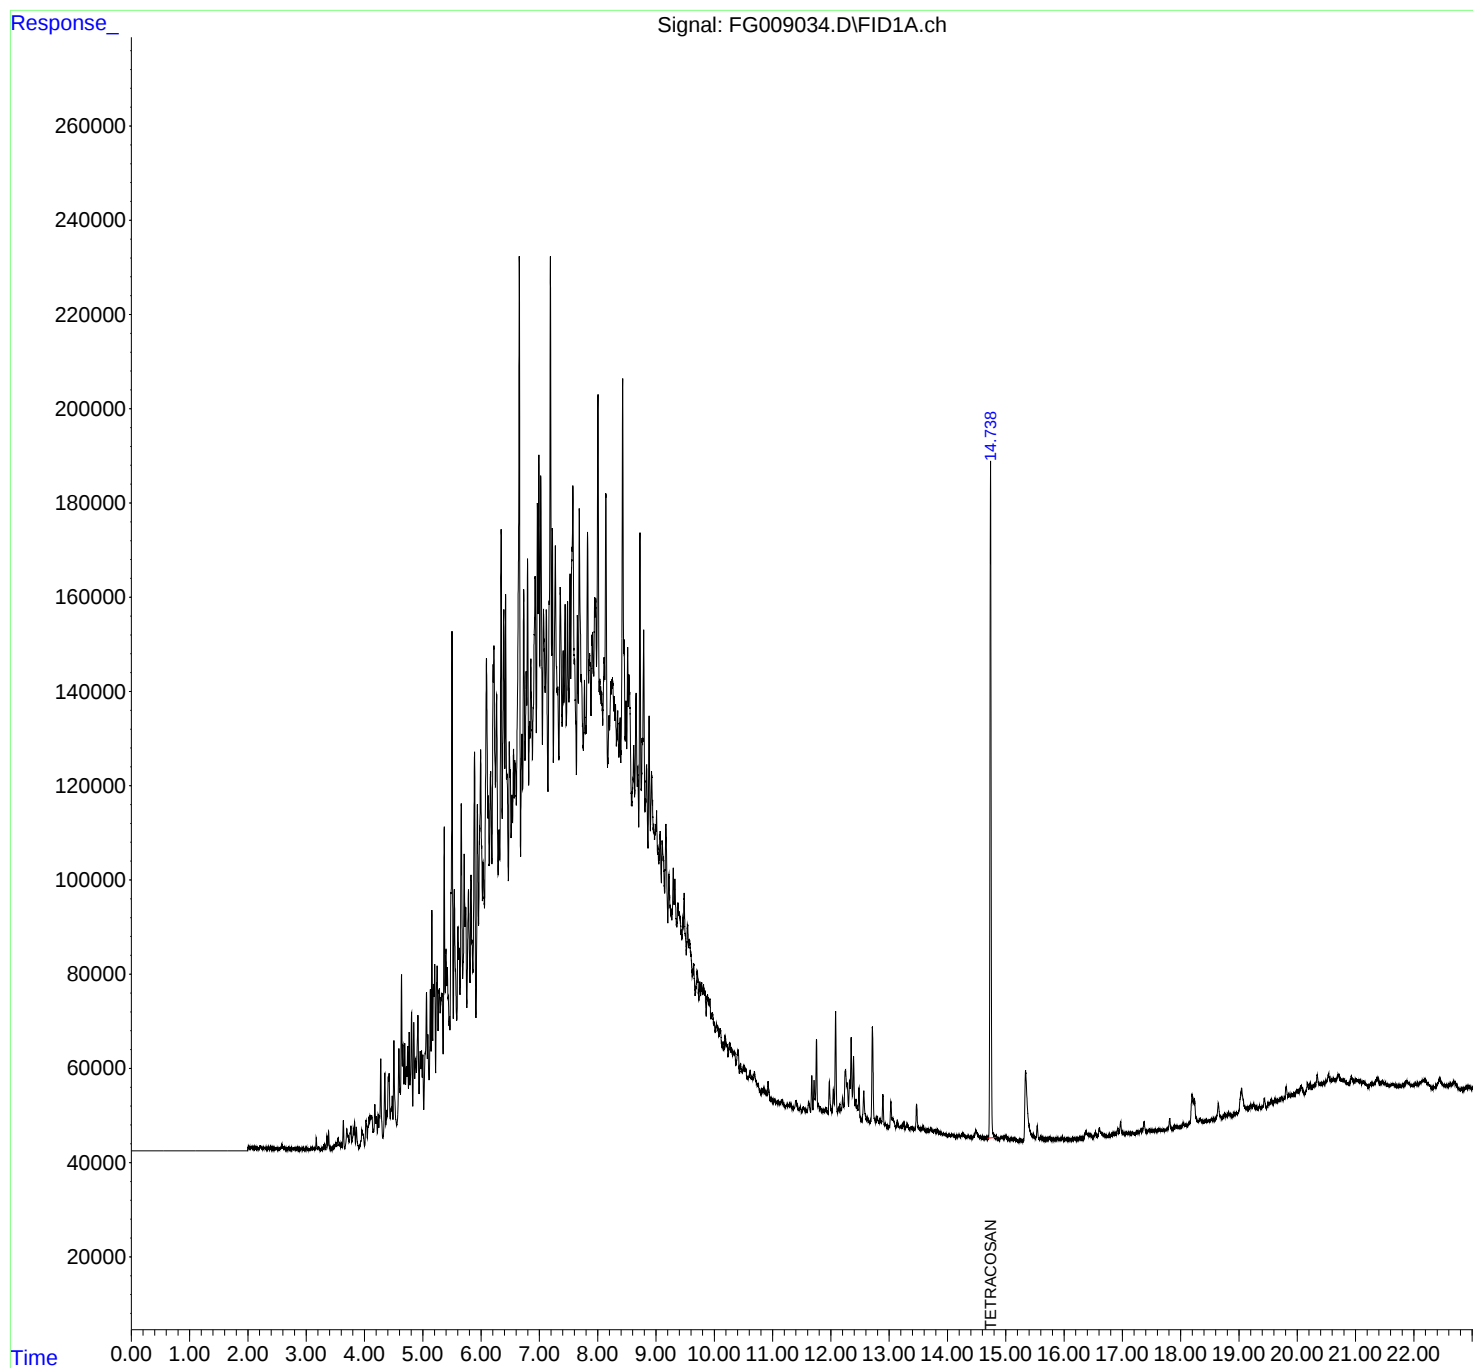

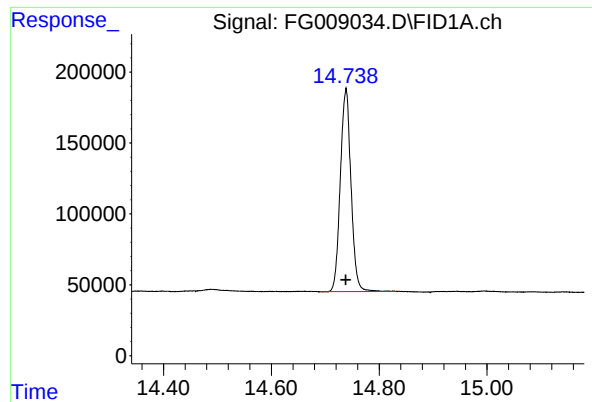

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.739 min
Delta R.T.: 0.000 min
Response: 1961523
Conc: 17.00 ug/ml

Instrument :

FID_G

ClientSampleId :

HB-1-(7.5-8)-11-11-21