

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111318\
 Data File : FG002922.D
 Signal(s) : FID1A.ch
 Acq On : 13 Nov 2018 19:03
 Operator : AJ\SJ
 Sample : J5909-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 14 03:55:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.752	2194929	19.972 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.349f	362569	2.742 ug/ml
10)	N-TETRACOSANE	14.952	118887	0.952 ug/ml
11)	N-HEXACOSANE	15.975	165195	1.340 ug/ml
12)	N-OCTACOSANE	16.928	227948	1.874 ug/ml
13)	N-TRIACONTANE	17.818	240885	2.008 ug/ml
14)	N-DOTRIACONTANE	18.652	131929	1.144 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111318\
Data File : FG002922.D
Signal(s) : FID1A.ch
Acq On : 13 Nov 2018 19:03
Operator : AJ\SJ
Sample : J5909-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 14 03:55:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

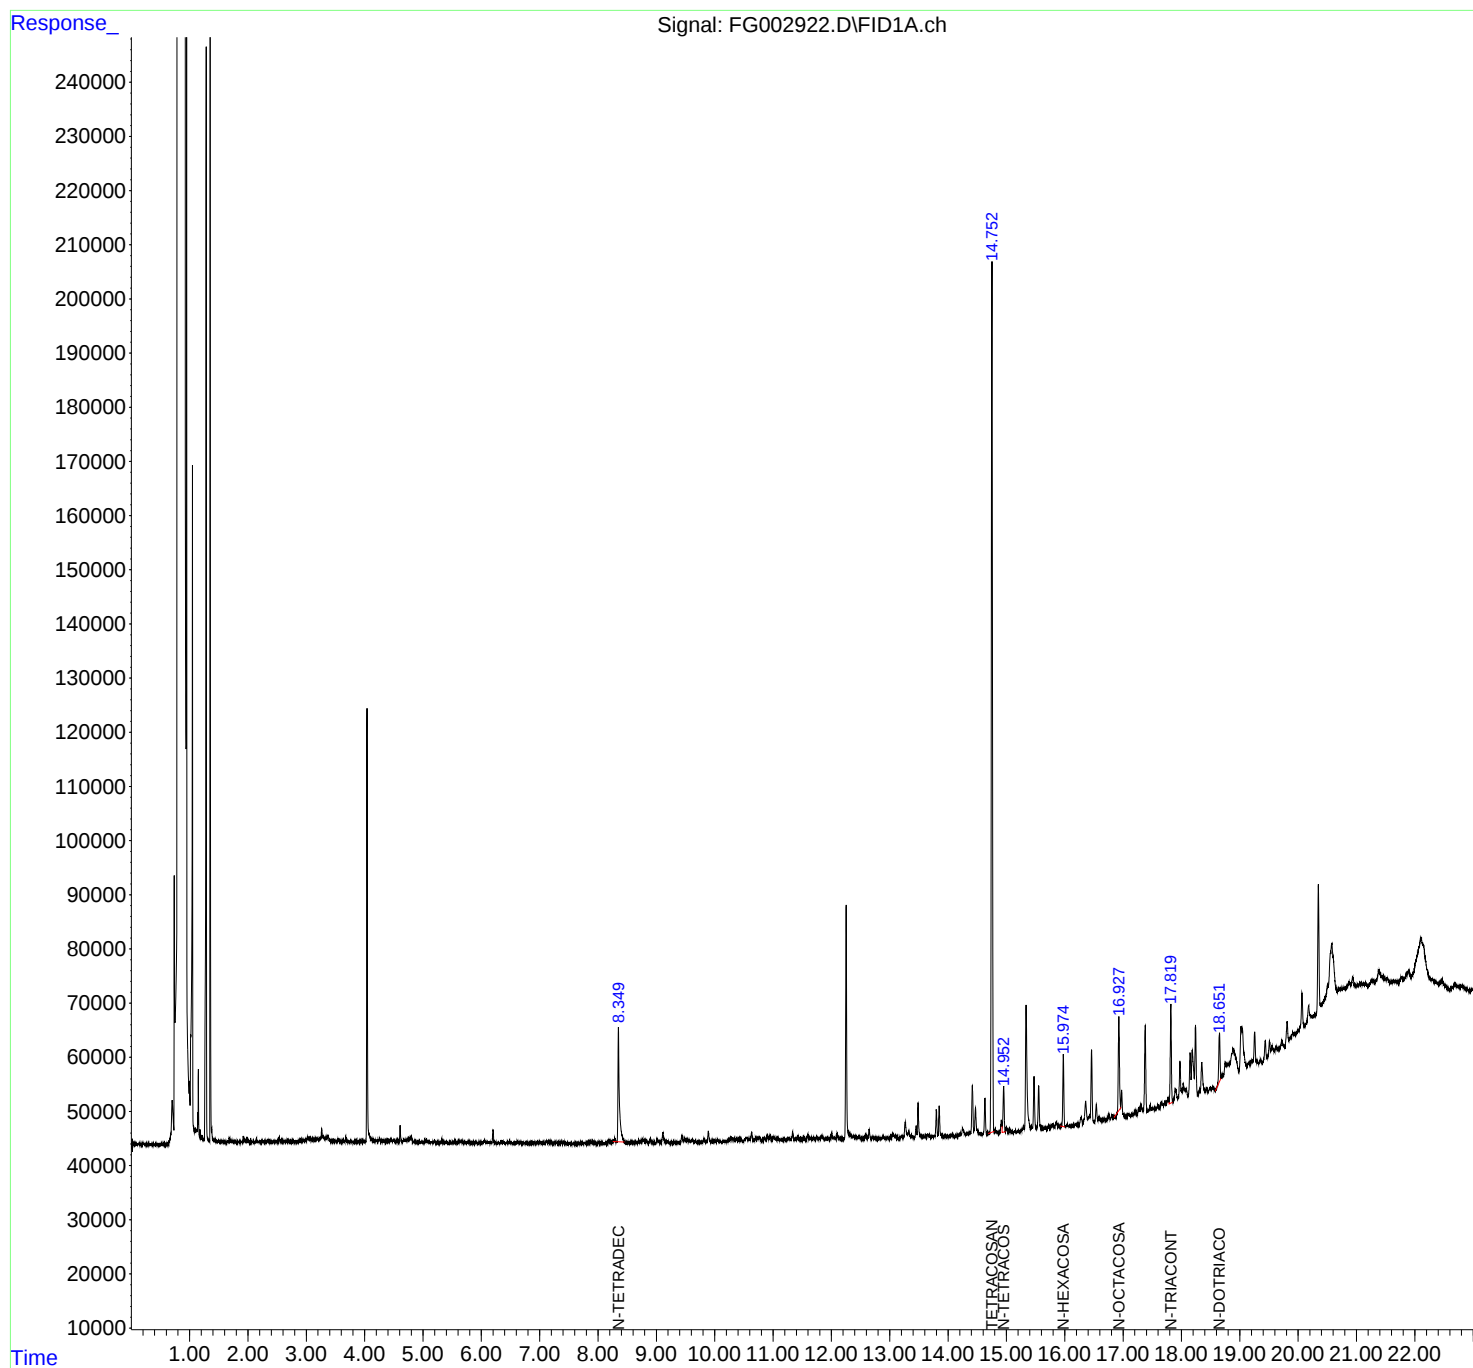

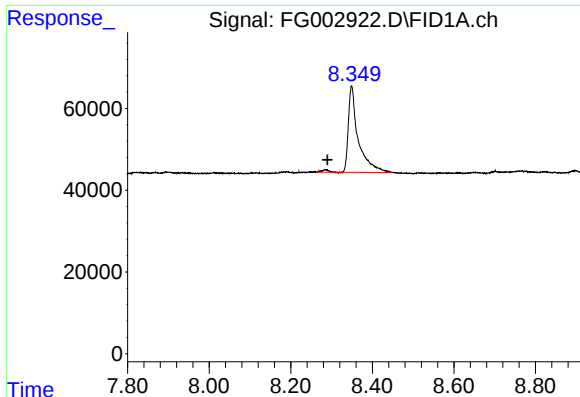


#4 N-TETRADECANE

R.T.: 8.349 min
Delta R.T.: 0.060 min
Response: 362569
Conc: 2.74 ug/ml

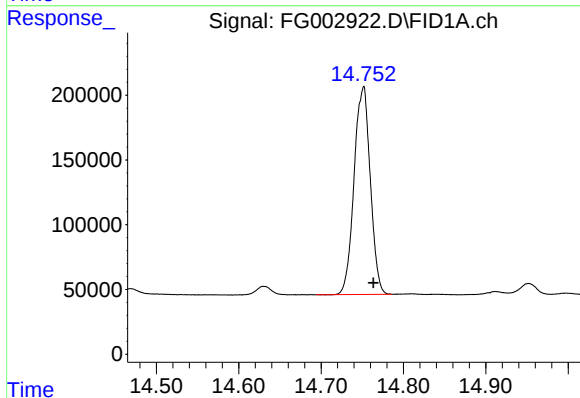


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.752 min
Delta R.T.: -0.012 min
Response: 2194929
Conc: 19.97 ug/ml

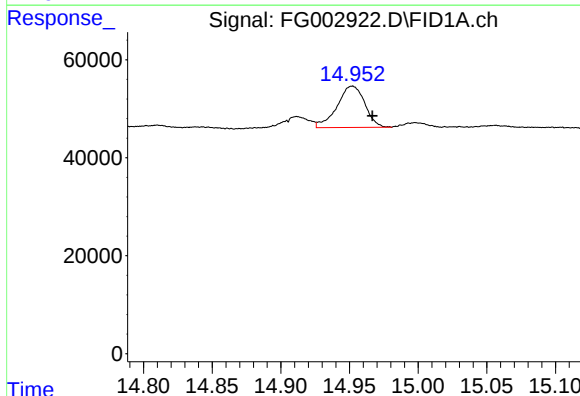


#10 N-TETRACOSANE

R.T.: 14.952 min
Delta R.T.: -0.015 min
Response: 118887
Conc: 0.95 ug/ml

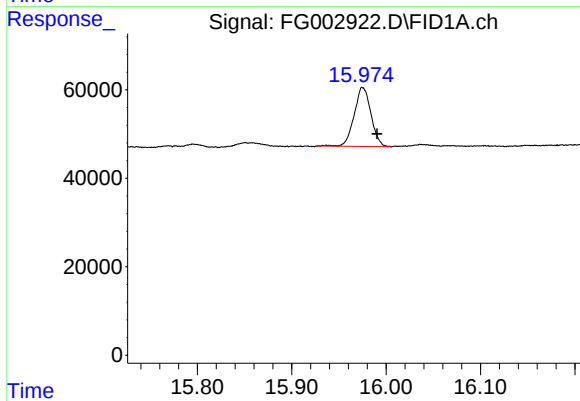


#11 N-HEXACOSANE

R.T.: 15.975 min
Delta R.T.: -0.015 min
Response: 165195
Conc: 1.34 ug/ml

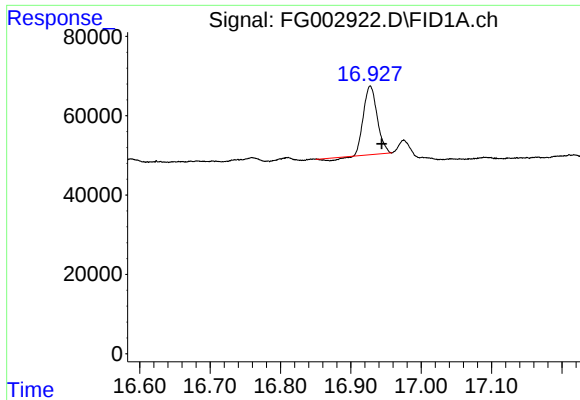


#12 N-OCTACOSANE

R.T.: 16.928 min
Delta R.T.: -0.016 min
Response: 227948
Conc: 1.87 ug/ml

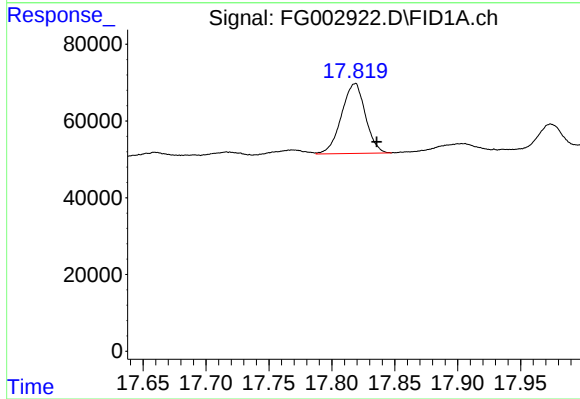

#13 N-TRIACONTANE

R.T.: 17.818 min
Delta R.T.: -0.017 min
Response: 240885
Conc: 2.01 ug/ml

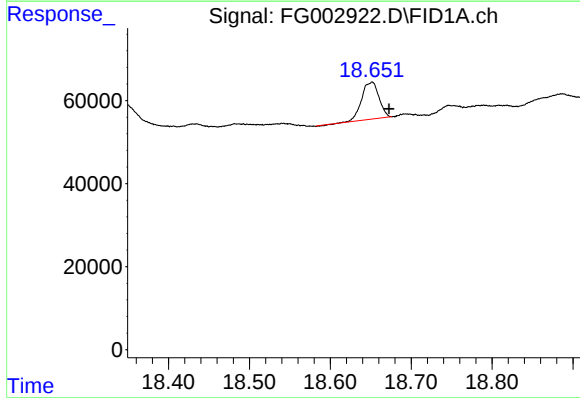

#14 N-DOTRIACONTANE

R.T.: 18.652 min
Delta R.T.: -0.021 min
Response: 131929
Conc: 1.14 ug/ml