

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111318\
 Data File : FG002942.D
 Signal(s) : FID1A.ch
 Acq On : 14 Nov 2018 05:11
 Operator : AJ\SJ
 Sample : J5908-17
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 14 07:56:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.754	3093030	28.144 ug/ml
Target Compounds			
4) N-TETRADECANE	8.348f	602116	4.554 ug/ml
7) N-EICOSANE	12.647	70551	0.544 ug/ml
8) N-DOCOSANE	13.854	965297	7.583 ug/ml
10) N-TETRACOSANE	14.952	1364934	10.926 ug/ml
11) N-HEXACOSANE	15.979	695679	5.645 ug/ml
12) N-OCTACOSANE	16.932	806728	6.633 ug/ml
13) N-TRIACONTANE	17.819	513710	4.281 ug/ml
14) N-DOTRIACONTANE	18.652	379747	3.294 ug/ml
15) N-TETRATRIACONTANE	19.475	203535	1.830 ug/ml
16) N-HEXATRIACONTANE	20.203	160129	1.521 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111318\
Data File : FG002942.D
Signal(s) : FID1A.ch
Acq On : 14 Nov 2018 05:11
Operator : AJ\SJ
Sample : J5908-17
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 14 07:56:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

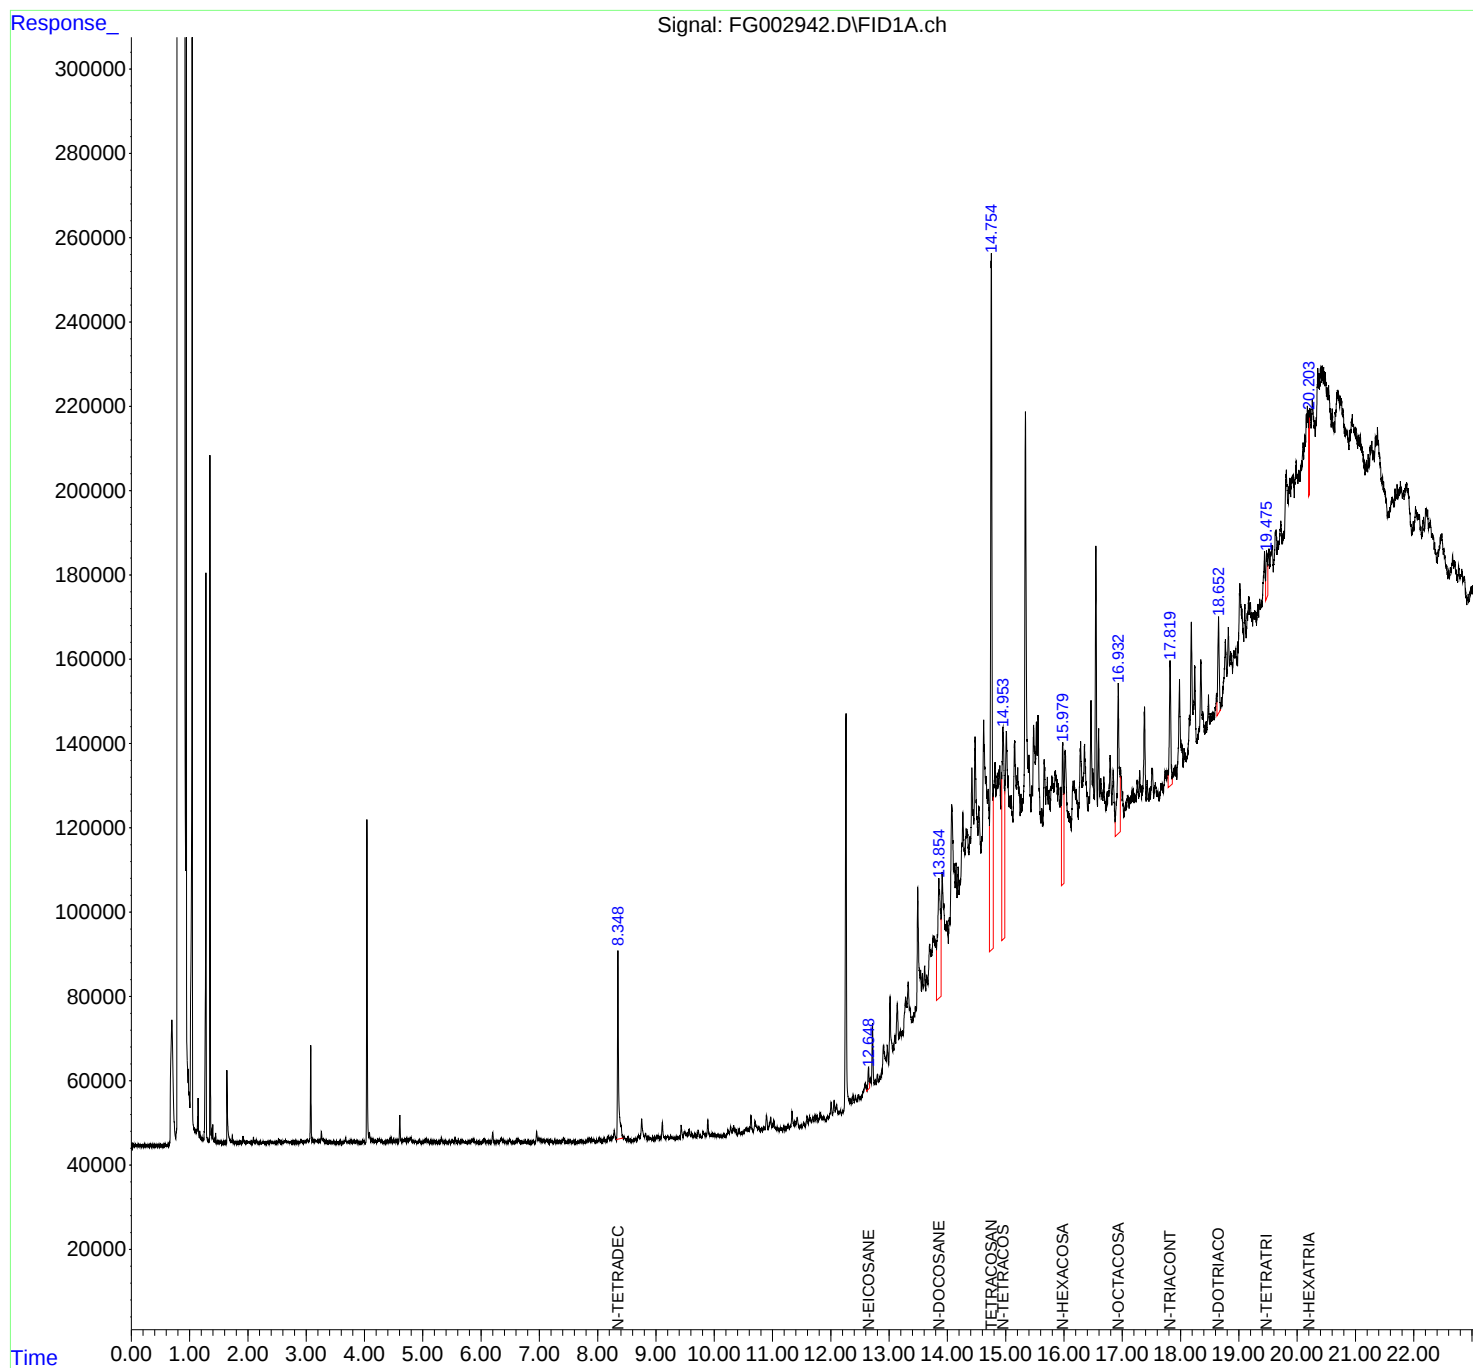

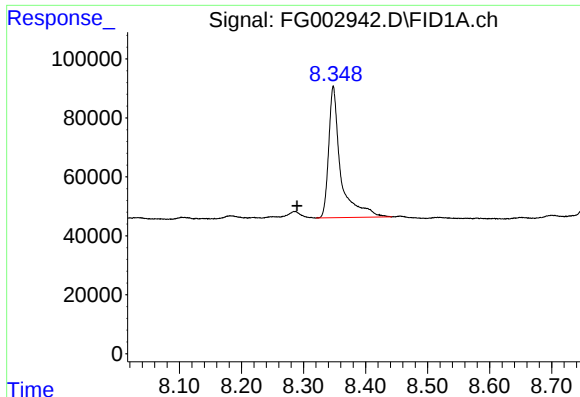


#4 N-TETRADECANE

R.T.: 8.348 min
Delta R.T.: 0.058 min
Response: 602116
Conc: 4.55 ug/ml

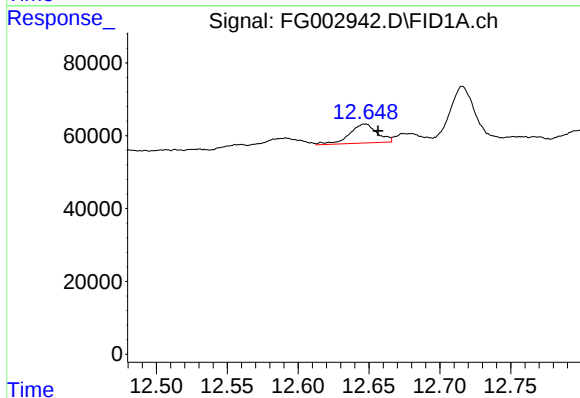


#7 N-EICOSANE

R.T.: 12.647 min
Delta R.T.: -0.009 min
Response: 70551
Conc: 0.54 ug/ml

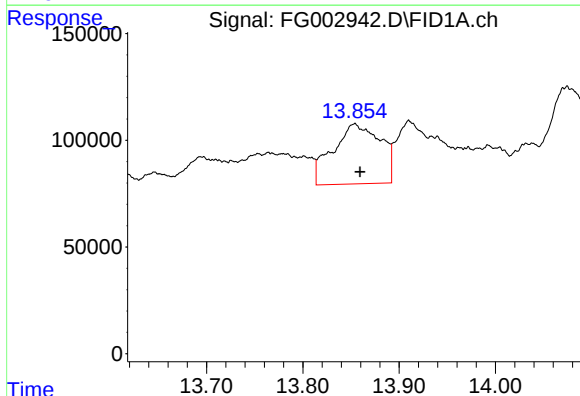


#8 N-DOCOSANE

R.T.: 13.854 min
Delta R.T.: -0.006 min
Response: 965297
Conc: 7.58 ug/ml

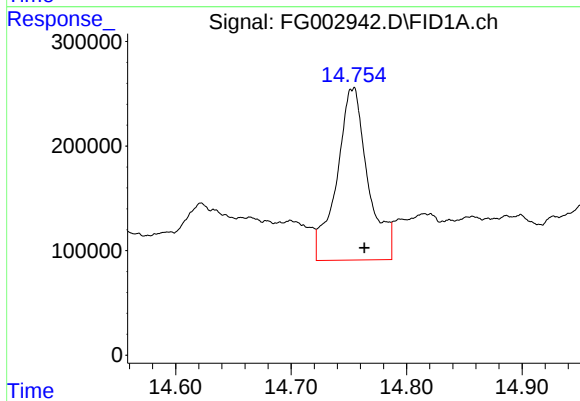


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.754 min
Delta R.T.: -0.010 min
Response: 3093030
Conc: 28.14 ug/ml

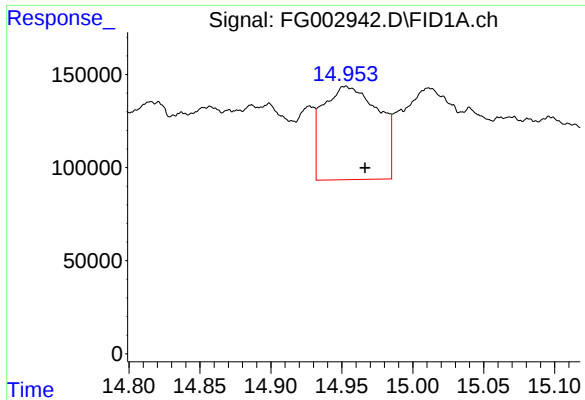


#10 N-TETRACOSANE

R.T.: 14.952 min
Delta R.T.: -0.014 min
Response: 1364934
Conc: 10.93 ug/ml

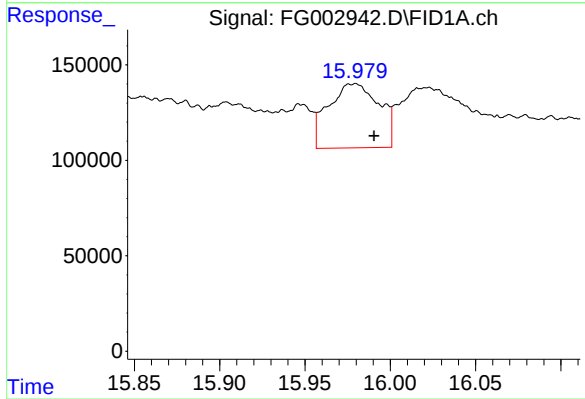


#11 N-HEXACOSANE

R.T.: 15.979 min
Delta R.T.: -0.011 min
Response: 695679
Conc: 5.64 ug/ml

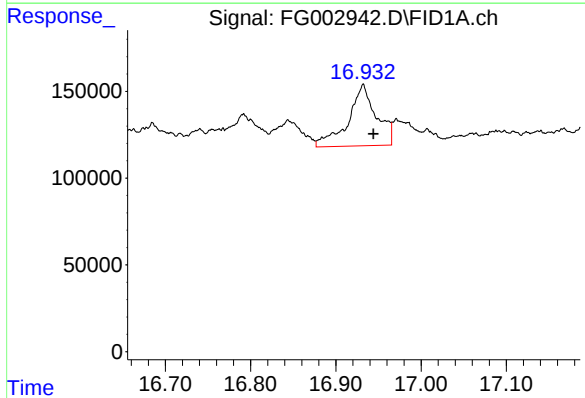


#12 N-OCTACOSANE

R.T.: 16.932 min
Delta R.T.: -0.012 min
Response: 806728
Conc: 6.63 ug/ml

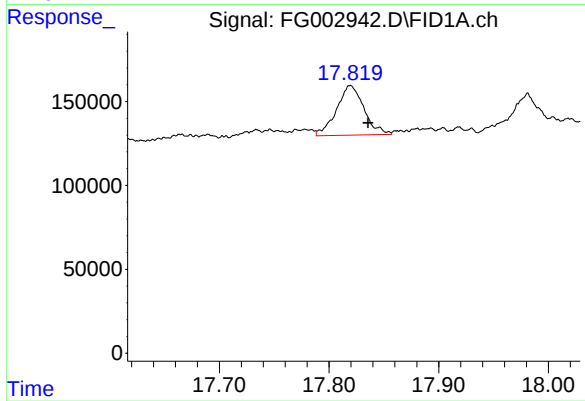


#13 N-TRIACONTANE

R.T.: 17.819 min
Delta R.T.: -0.016 min
Response: 513710
Conc: 4.28 ug/ml

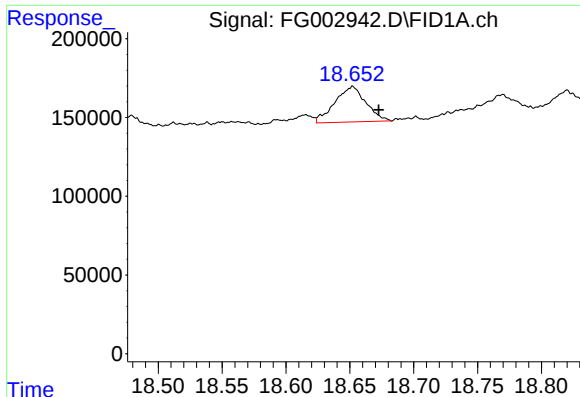


#14 N-DOTRIACONTANE

R.T.: 18.652 min
Delta R.T.: -0.020 min
Response: 379747
Conc: 3.29 ug/ml

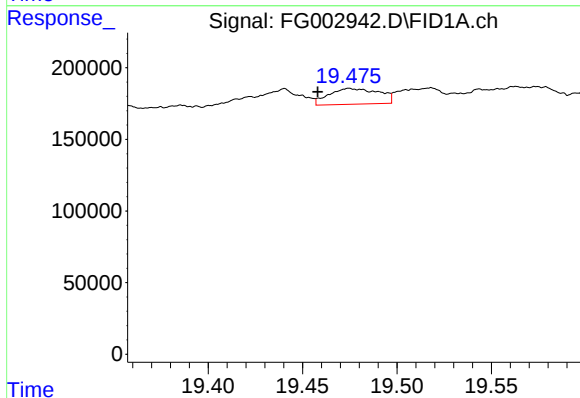

#15 N-TETRATRIACONTANE

R.T.: 19.475 min
Delta R.T.: 0.017 min
Response: 203535
Conc: 1.83 ug/ml

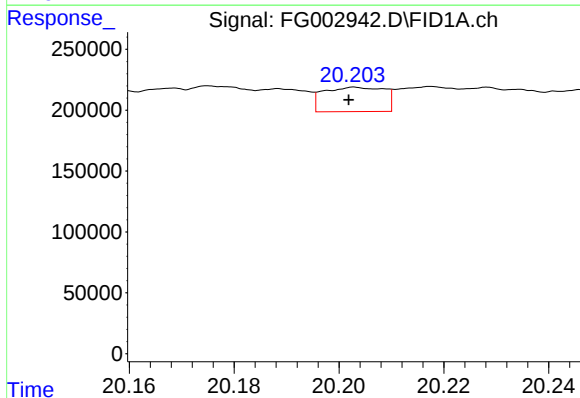

#16 N-HEXATRIACONTANE

R.T.: 20.203 min
Delta R.T.: 0.002 min
Response: 160129
Conc: 1.52 ug/ml