

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111318\
Data File : FG002944.D
Signal(s) : FID1A.ch
Acq On : 14 Nov 2018 06:11
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 14 07:57:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.750	1993041	18.135 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.816	116959	0.975 ug/ml
14)	N-DOTRIACONTANE	18.650	184176	1.598 ug/ml
15)	N-TETRATRIACONTANE	19.434	136371	1.226 ug/ml
16)	N-HEXATRIACONTANE	20.202	186649	1.773 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111318\
Data File : FG002944.D
Signal(s) : FID1A.ch
Acq On : 14 Nov 2018 06:11
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 14 07:57:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

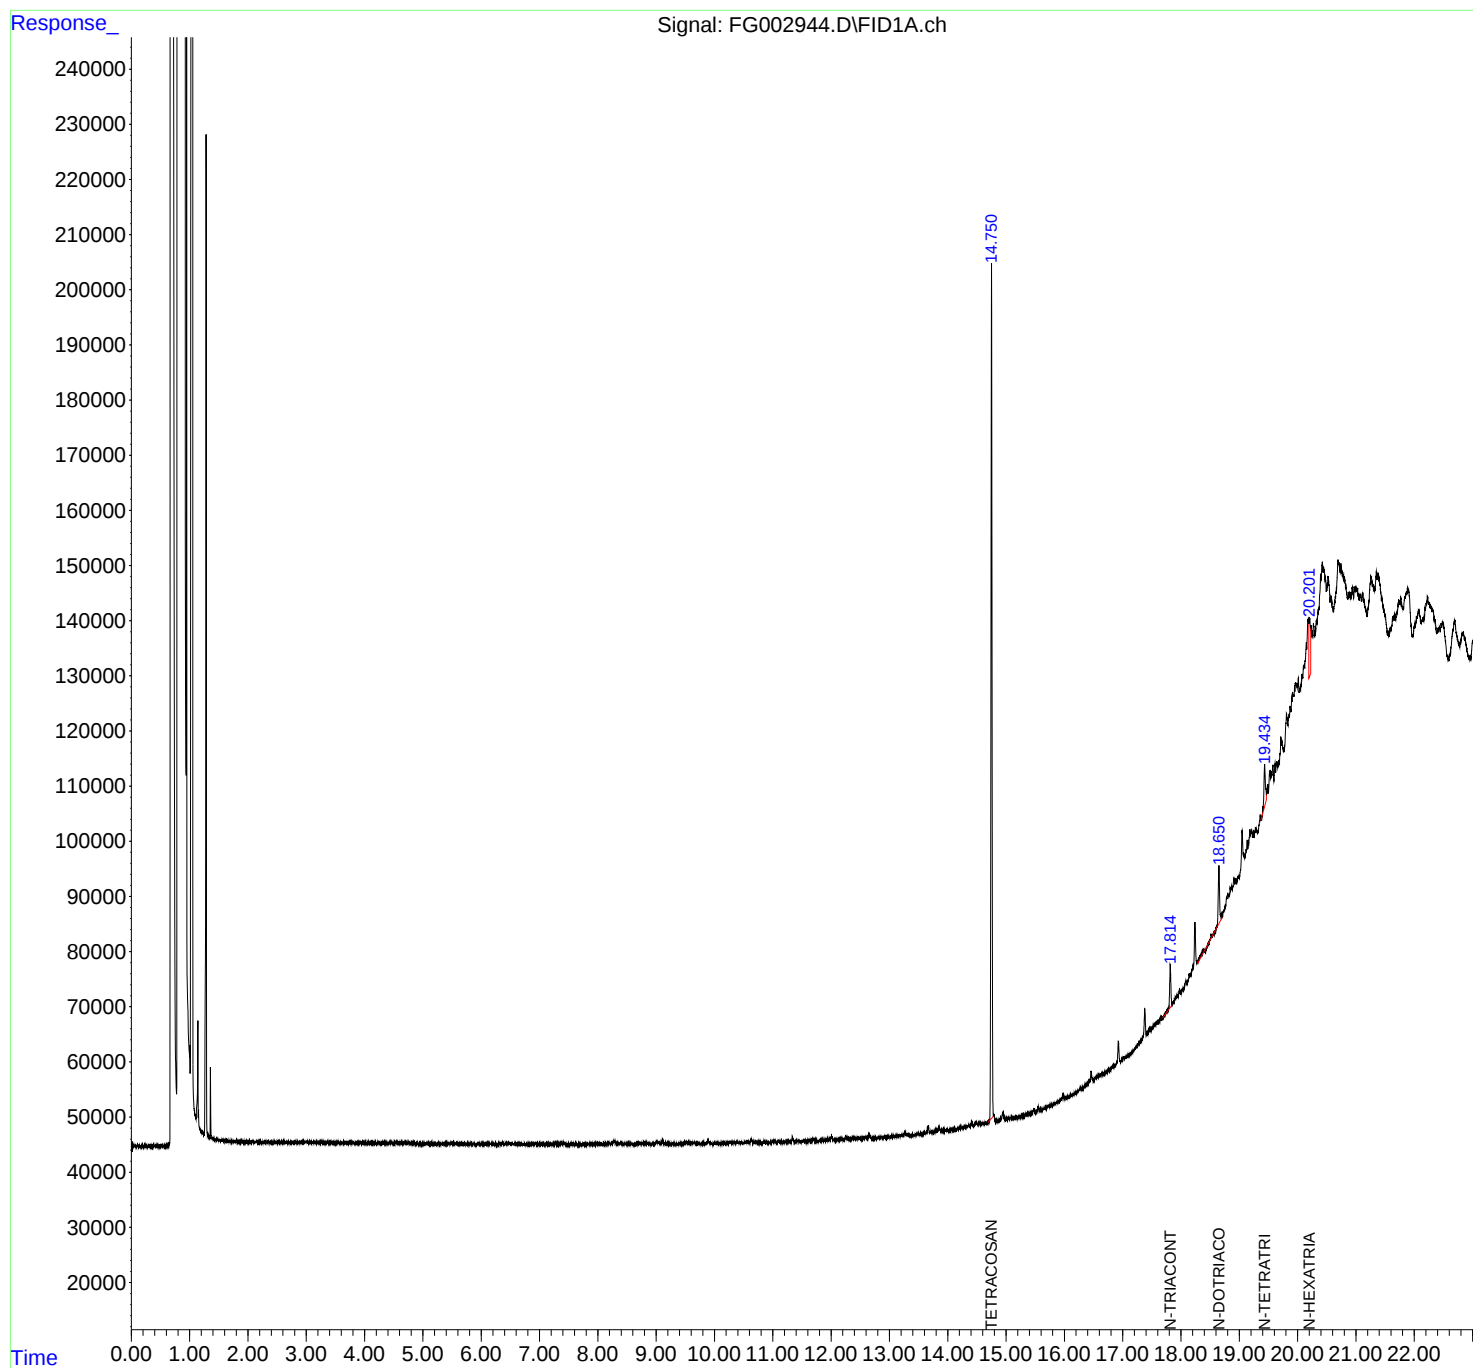

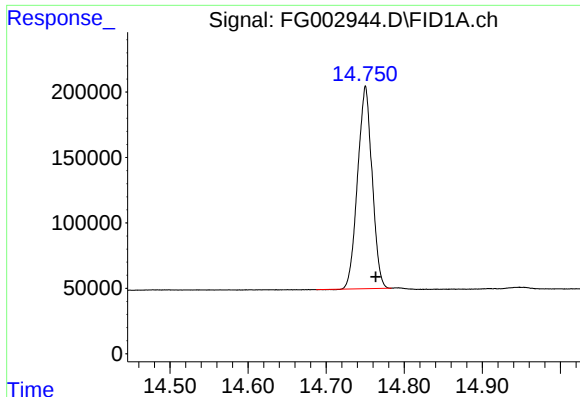


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: -0.013 min
Response: 1993041
Conc: 18.13 ug/ml

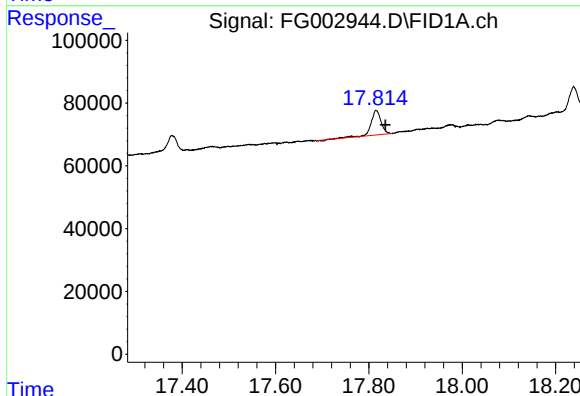


#13 N-TRIACONTANE

R.T.: 17.816 min
Delta R.T.: -0.020 min
Response: 116959
Conc: 0.97 ug/ml

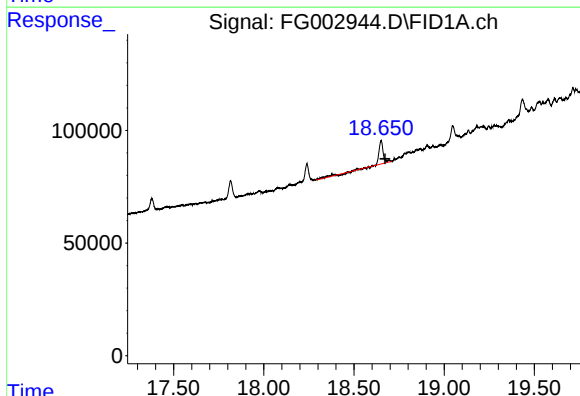


#14 N-DOTRIACONTANE

R.T.: 18.650 min
Delta R.T.: -0.022 min
Response: 184176
Conc: 1.60 ug/ml

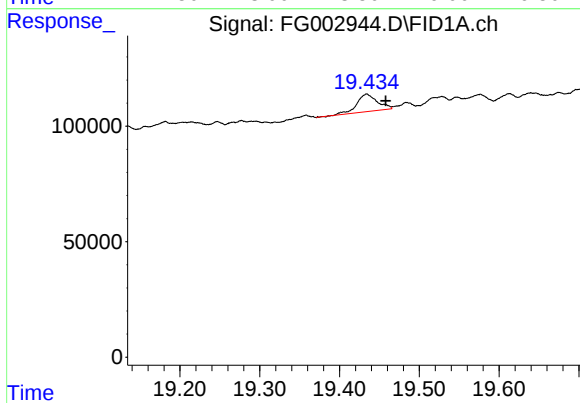

#15 N-TETRATRIACONTANE

R.T.: 19.434 min
Delta R.T.: -0.024 min
Response: 136371
Conc: 1.23 ug/ml

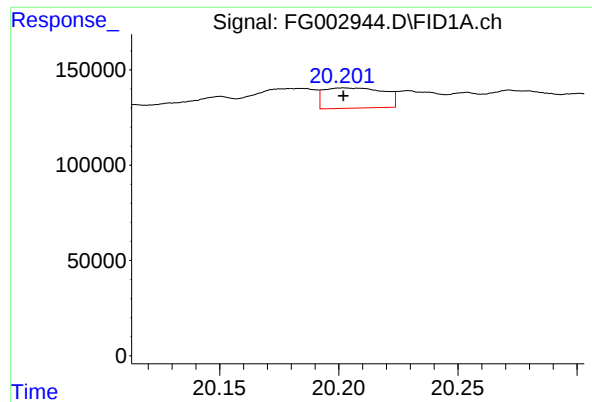

#16 N-HEXATRIACONTANE

R.T.: 20.202 min
Delta R.T.: 0.000 min
Response: 186649
Conc: 1.77 ug/ml