

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111318\
 Data File : FG002927.D
 Signal(s) : FID1A.ch
 Acq On : 13 Nov 2018 21:35
 Operator : AJ\SJ
 Sample : J5908-01MSD 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 14 03:56:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	387103	3.522 ug/ml
Target Compounds			
2) N-DECANE	4.458	416180	3.263 ug/ml
3) N-DODECANE	6.487	424454	3.256 ug/ml
4) N-TETRADECANE	8.286	432877	3.274 ug/mlm
5) N-HEXADECANE	9.890	464515	3.488 ug/mlm
6) N-OCTADECANE	11.335	447669	3.384 ug/ml
7) N-EICOSANE	12.647	455919	3.517 ug/ml
8) N-DOCOSANE	13.847	424050	3.331 ug/ml
10) N-TETRACOSANE	14.947	744573	5.960 ug/ml
11) N-HEXACOSANE	15.977	477198	3.872 ug/ml
12) N-OCTACOSANE	16.928	566958	4.661 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111318\
Data File : FG002927.D
Signal(s) : FID1A.ch
Acq On : 13 Nov 2018 21:35
Operator : AJ\SJ
Sample : J5908-01MSD 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 14 03:56:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

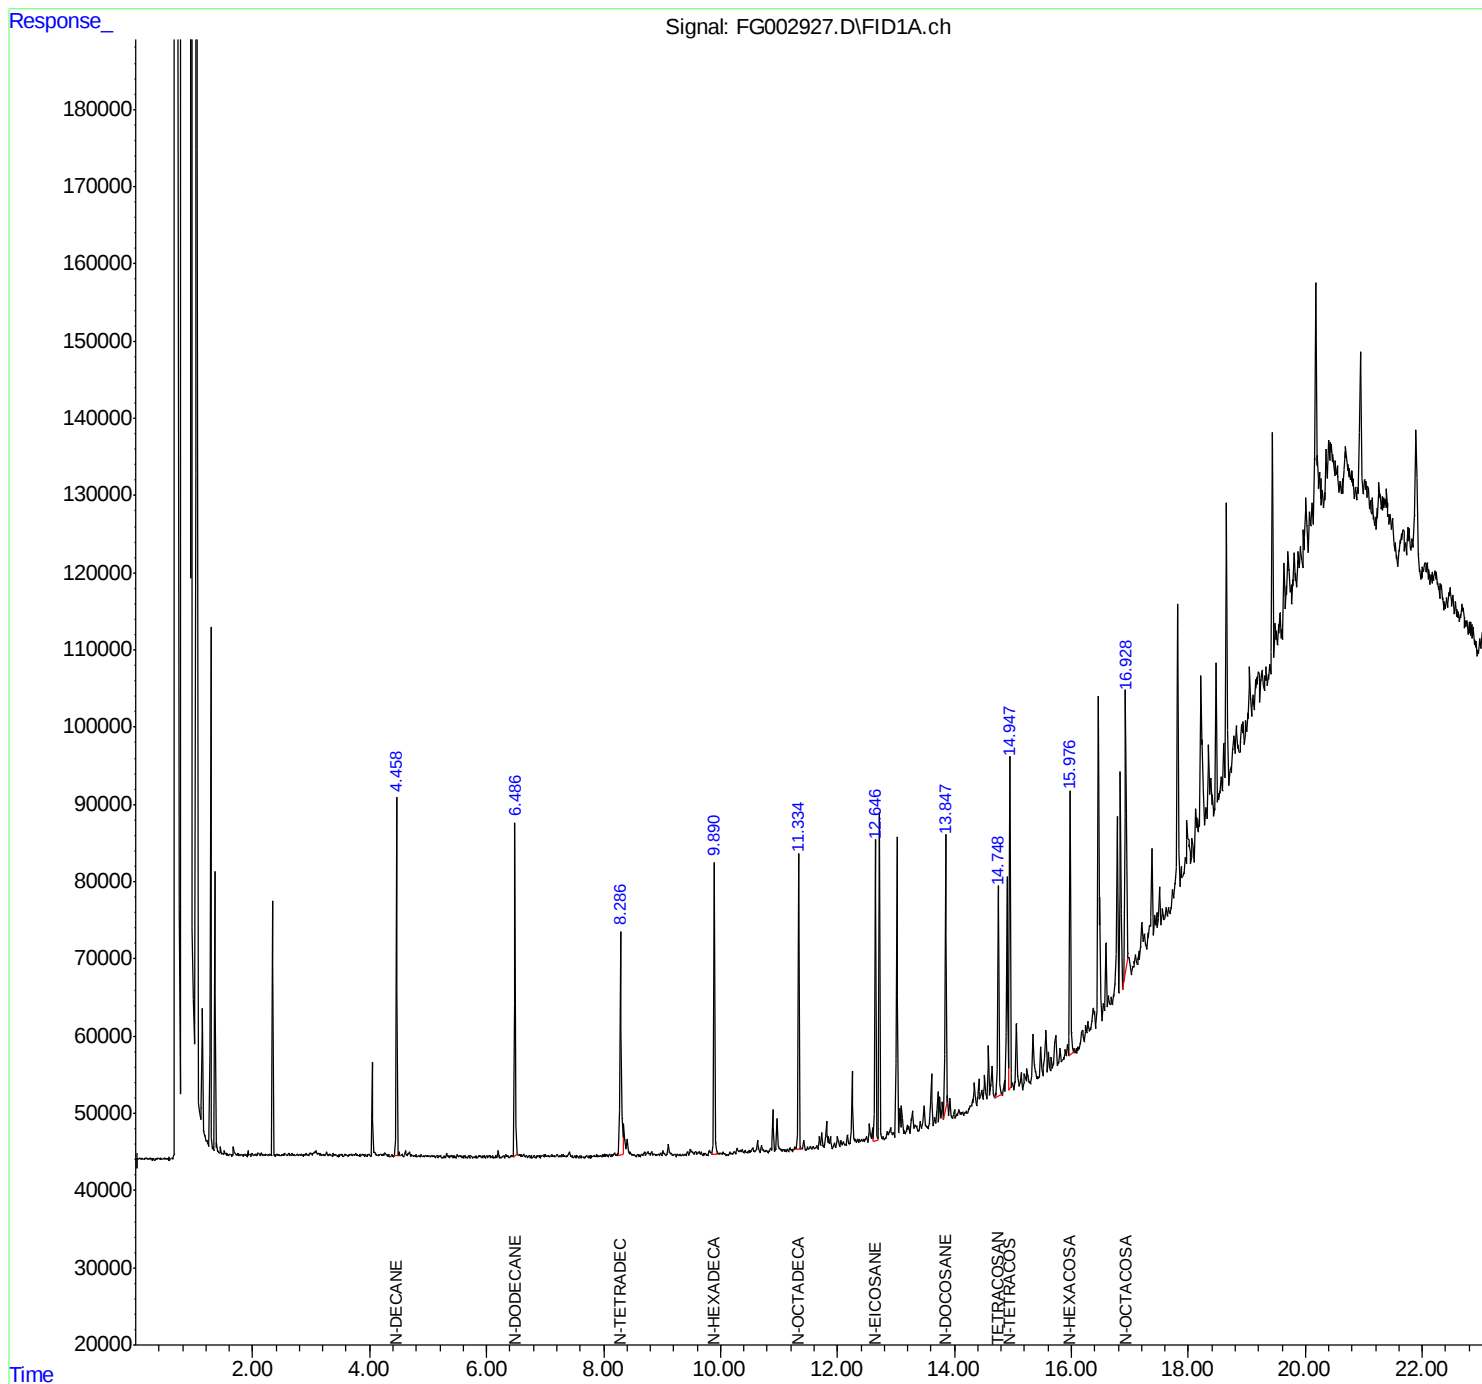

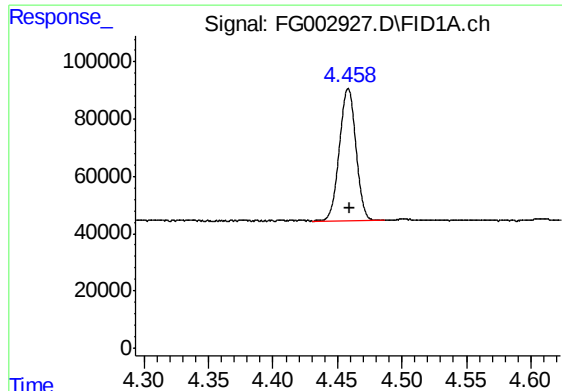


#2 N-DECANE

R.T.: 4.458 min
Delta R.T.: 0.000 min
Response: 416180
Conc: 3.26 ug/ml

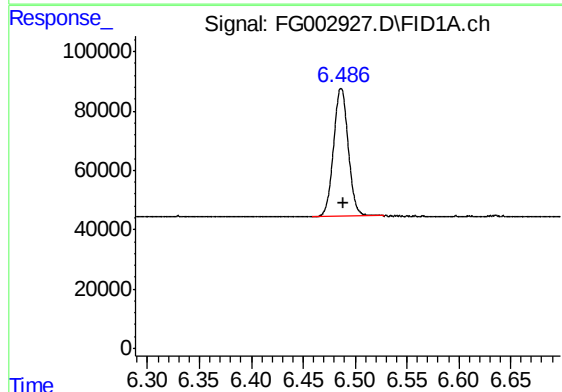


#3 N-DODECANE

R.T.: 6.487 min
Delta R.T.: -0.002 min
Response: 424454
Conc: 3.26 ug/ml

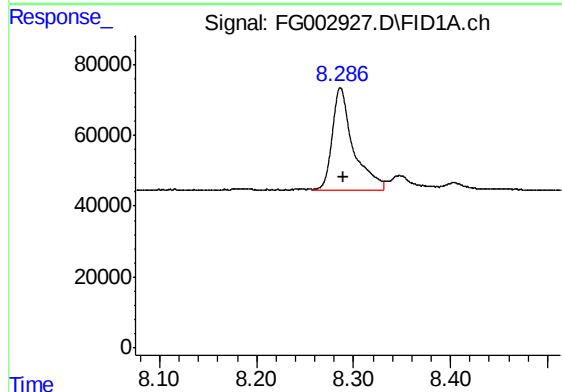


#4 N-TETRADECANE

R.T.: 8.286 min
Delta R.T.: -0.004 min
Response: 432877
Conc: 3.27 ug/ml m

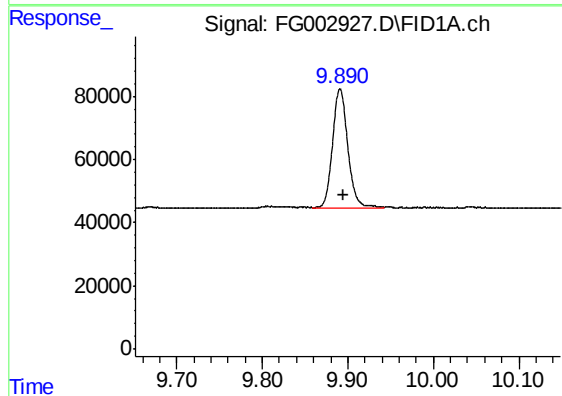


#5 N-HEXADECANE

R.T.: 9.890 min
Delta R.T.: -0.005 min
Response: 464515
Conc: 3.49 ug/ml m

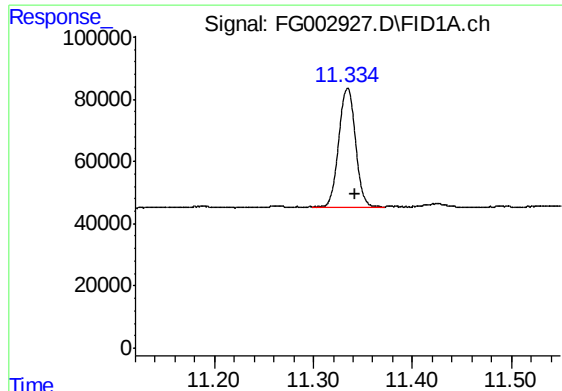


#6 N-OCTADECANE

R.T.: 11.335 min
Delta R.T.: -0.007 min
Response: 447669
Conc: 3.38 ug/ml

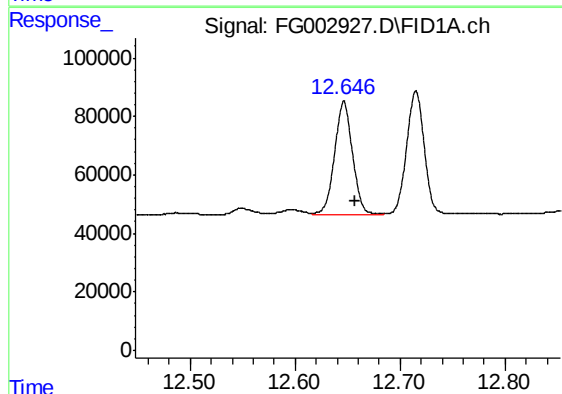


#7 N-EICOSANE

R.T.: 12.647 min
Delta R.T.: -0.010 min
Response: 455919
Conc: 3.52 ug/ml

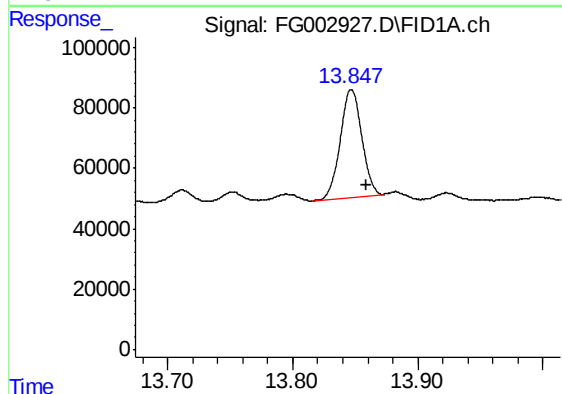


#8 N-DOCOSANE

R.T.: 13.847 min
Delta R.T.: -0.012 min
Response: 424050
Conc: 3.33 ug/ml

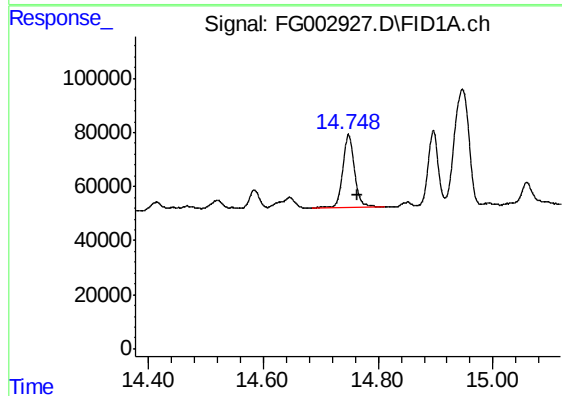


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.749 min
Delta R.T.: -0.015 min
Response: 387103
Conc: 3.52 ug/ml

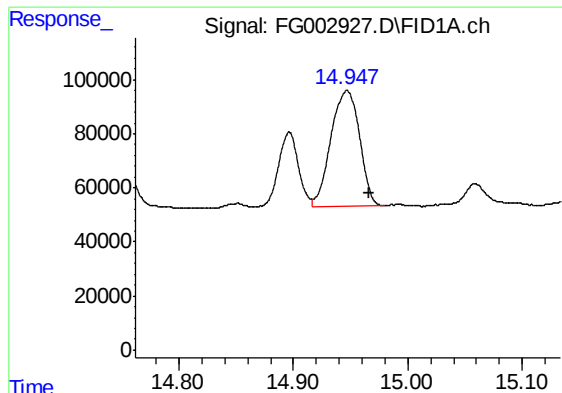


#10 N-TETRACOSANE

R.T.: 14.947 min
Delta R.T.: -0.019 min
Response: 744573
Conc: 5.96 ug/ml

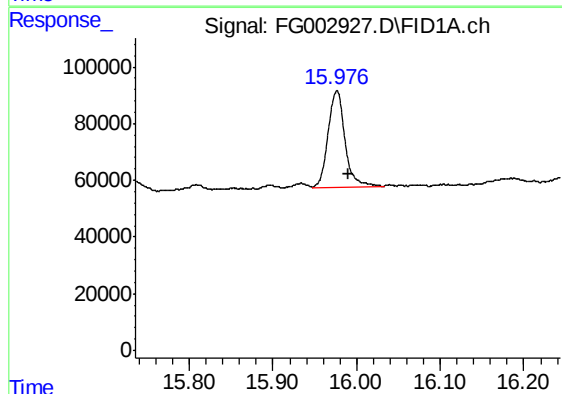

#11 N-HEXACOSANE

R.T.: 15.977 min
Delta R.T.: -0.014 min
Response: 477198
Conc: 3.87 ug/ml

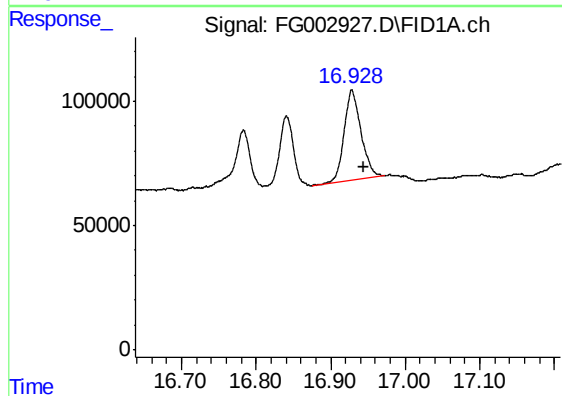

#12 N-OCTACOSANE

R.T.: 16.928 min
Delta R.T.: -0.016 min
Response: 566958
Conc: 4.66 ug/ml