

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111418\
 Data File : FG002959.D
 Signal(s) : FID1A.ch
 Acq On : 14 Nov 2018 17:01
 Operator : AJ\SJ
 Sample : J5910-01MSD 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 15 01:12:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	444244	4.042 ug/mlm
Target Compounds			
2) N-DECANE	4.458	518996	4.069 ug/ml
3) N-DODECANE	6.486	525443	4.031 ug/ml
4) N-TETRADECANE	8.285	515177	3.896 ug/mlm
5) N-HEXADECANE	9.889	552357	4.148 ug/ml
6) N-OCTADECANE	11.334	520135	3.932 ug/ml
7) N-EICOSANE	12.645	528765	4.079 ug/ml
8) N-DOCOSANE	13.845	510227	4.008 ug/mlm
10) N-TETRACOSANE	14.949	619346	4.958 ug/ml
11) N-HEXACOSANE	15.972	464258	3.767 ug/mlm
12) N-OCTACOSANE	16.923	525851	4.323 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111418\
Data File : FG002959.D
Signal(s) : FID1A.ch
Acq On : 14 Nov 2018 17:01
Operator : AJ\SJ
Sample : J5910-01MSD 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 15 01:12:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

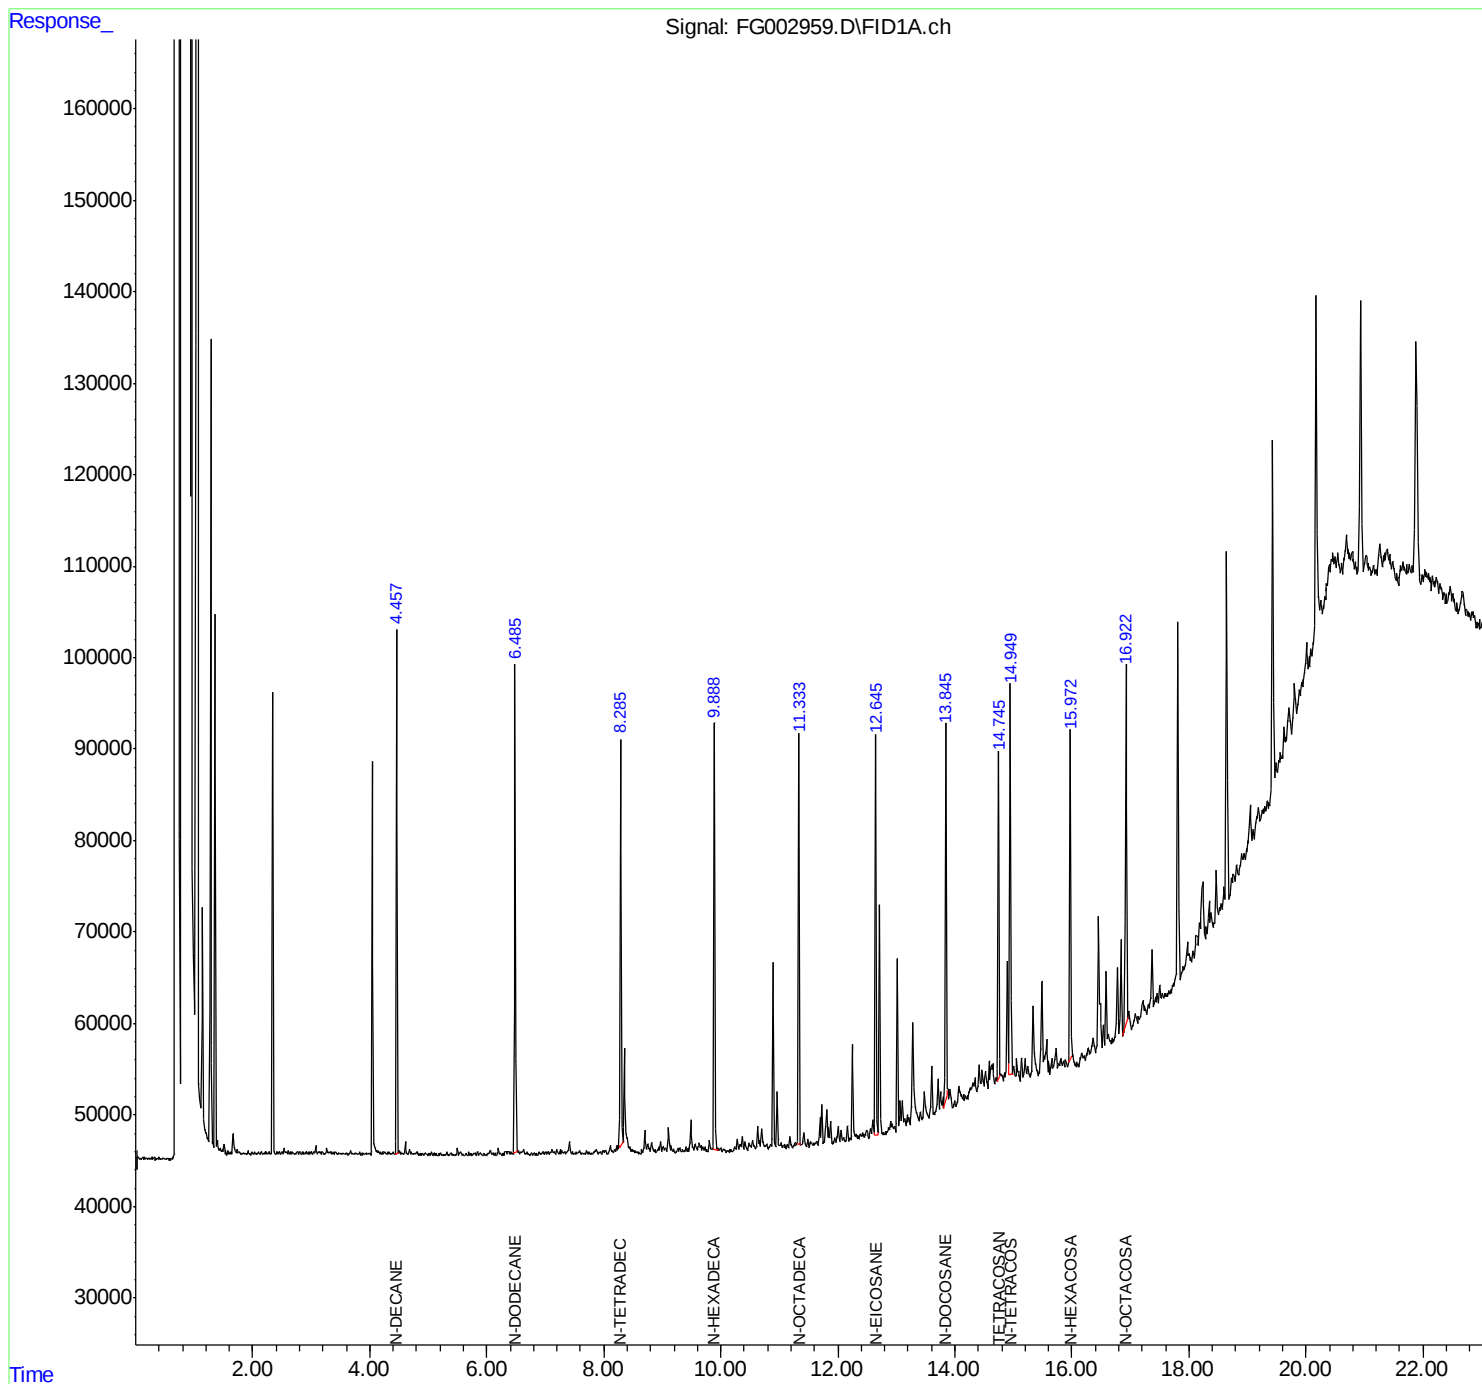

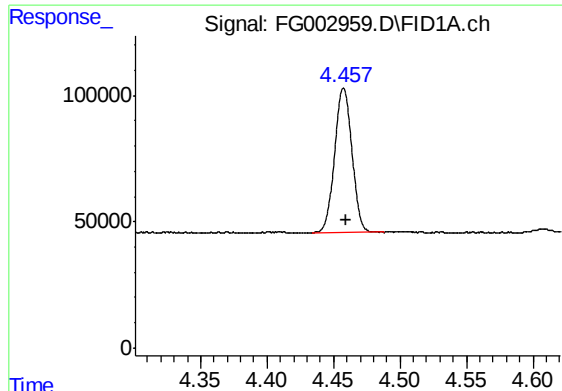


#2 N-DECANE

R.T.: 4.458 min
Delta R.T.: -0.002 min
Response: 518996
Conc: 4.07 ug/ml

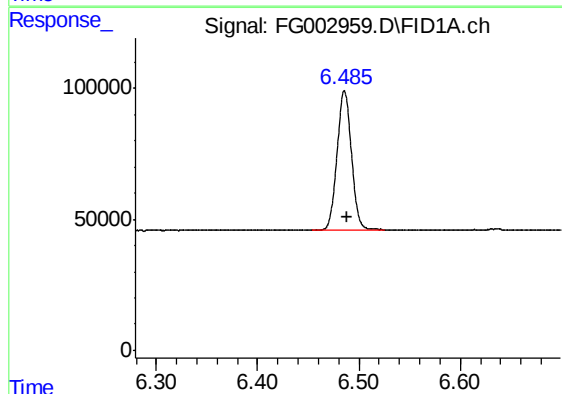


#3 N-DODECANE

R.T.: 6.486 min
Delta R.T.: -0.002 min
Response: 525443
Conc: 4.03 ug/ml

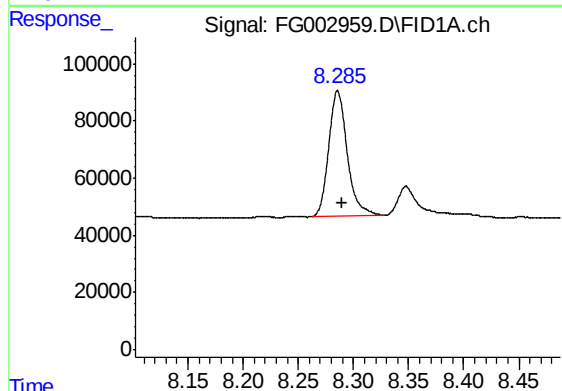


#4 N-TETRADECANE

R.T.: 8.285 min
Delta R.T.: -0.004 min
Response: 515177
Conc: 3.90 ug/ml m

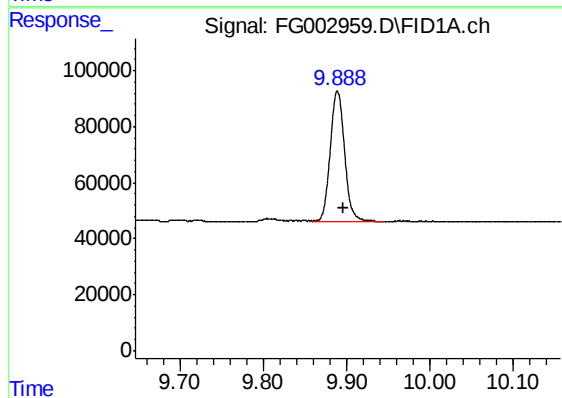


#5 N-HEXADECANE

R.T.: 9.889 min
Delta R.T.: -0.006 min
Response: 552357
Conc: 4.15 ug/ml

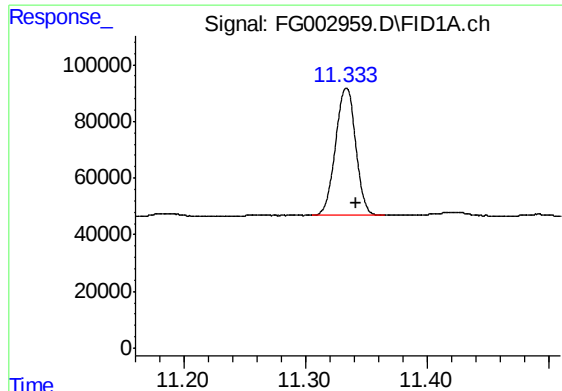


#6 N-OCTADECANE

R.T.: 11.334 min
Delta R.T.: -0.008 min
Response: 520135
Conc: 3.93 ug/ml

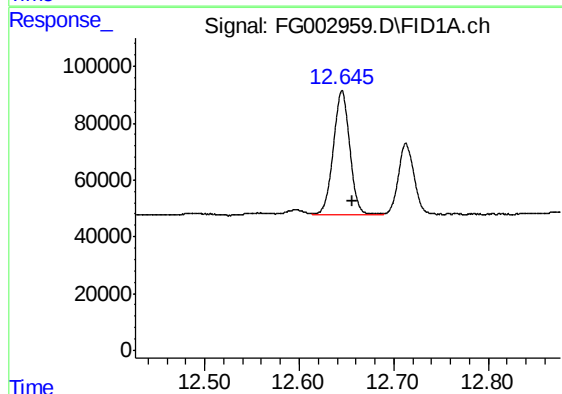


#7 N-EICOSANE

R.T.: 12.645 min
Delta R.T.: -0.011 min
Response: 528765
Conc: 4.08 ug/ml

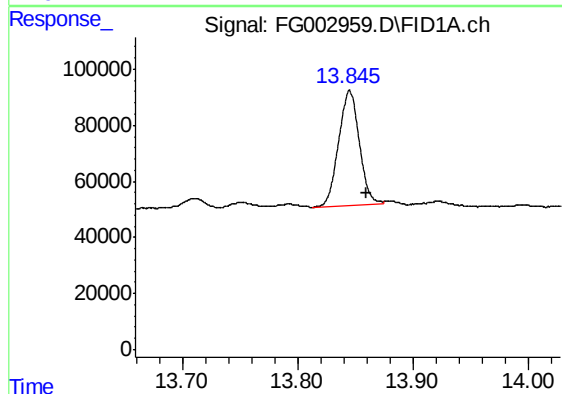


#8 N-DOCOSANE

R.T.: 13.845 min
Delta R.T.: -0.015 min
Response: 510227
Conc: 4.01 ug/ml m

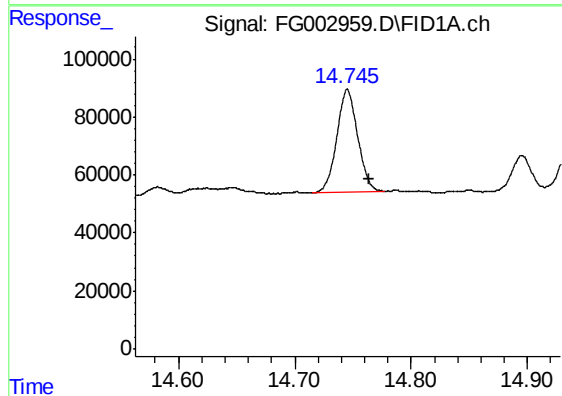


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.745 min
Delta R.T.: -0.019 min
Response: 444244
Conc: 4.04 ug/ml m

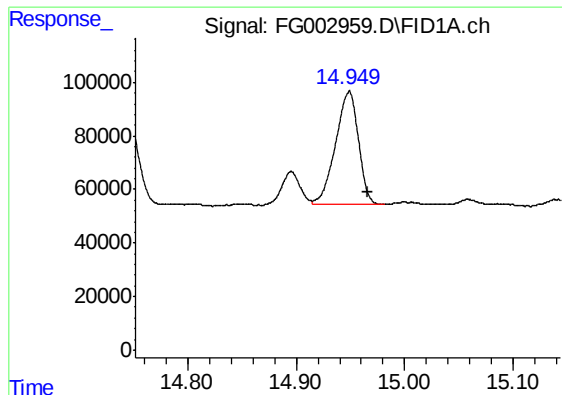


#10 N-TETRACOSANE

R.T.: 14.949 min
Delta R.T.: -0.018 min
Response: 619346
Conc: 4.96 ug/ml

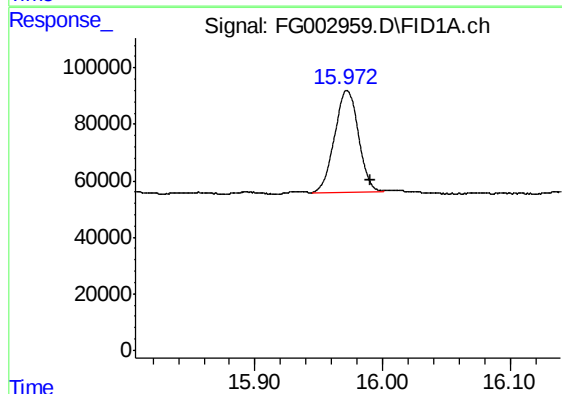

#11 N-HEXACOSANE

R.T.: 15.972 min
Delta R.T.: -0.019 min
Response: 464258
Conc: 3.77 ug/ml m

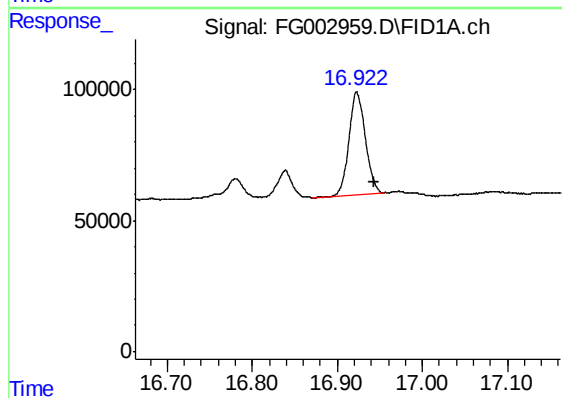

#12 N-OCTACOSANE

R.T.: 16.923 min
Delta R.T.: -0.021 min
Response: 525851
Conc: 4.32 ug/ml