

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111518\
 Data File : FG002971.D
 Signal(s) : FID1A.ch
 Acq On : 15 Nov 2018 11:18
 Operator : AJ\SJ
 Sample : J5925-06 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 15 16:00:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	130369	1.186 ug/ml
Target Compounds			
3) N-DODECANE	6.469	190053	1.458 ug/ml
4) N-TETRADECANE	8.278	452286	3.421 ug/ml
5) N-HEXADECANE	9.904	865307	6.498 ug/ml
6) N-OCTADECANE	11.326	363468	2.748 ug/ml
7) N-EICOSANE	12.636	376625	2.905 ug/ml
8) N-DOCOSANE	13.875	76435	0.600 ug/ml
10) N-TETRACOSANE	14.943	51483	0.412 ug/ml
11) N-HEXACOSANE	15.972	44321	0.360 ug/ml
12) N-OCTACOSANE	16.922	155970	1.282 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111518\
Data File : FG002971.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2018 11:18
Operator : AJ\SJ
Sample : J5925-06 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 15 16:00:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

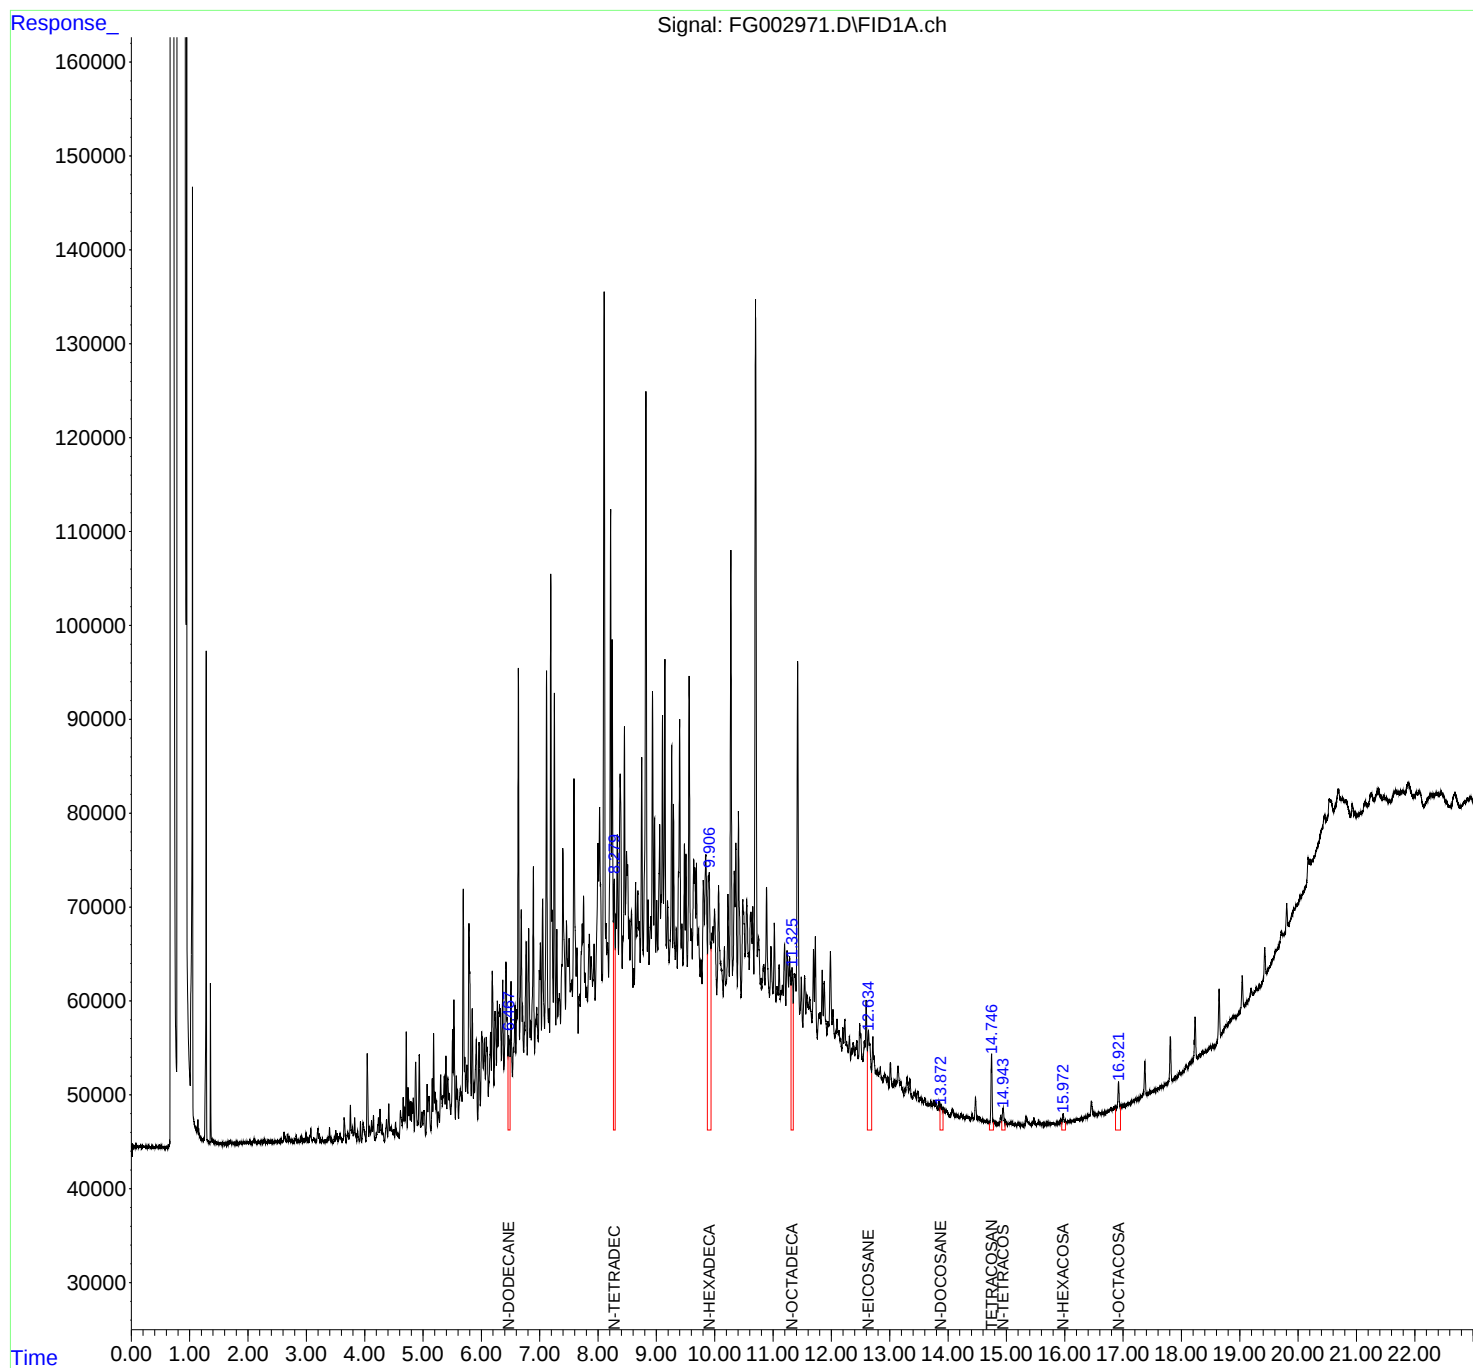

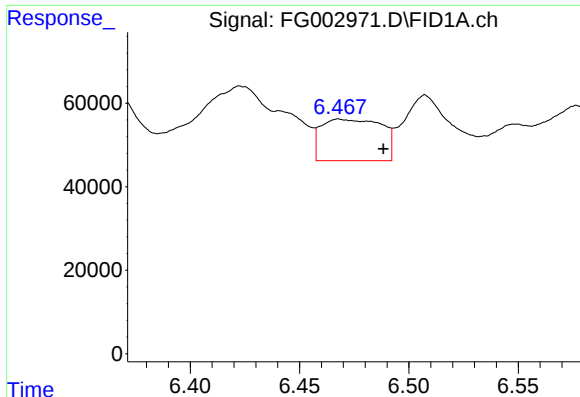


#3 N-DODECANE

R.T.: 6.469 min
Delta R.T.: -0.019 min
Response: 190053
Conc: 1.46 ug/ml

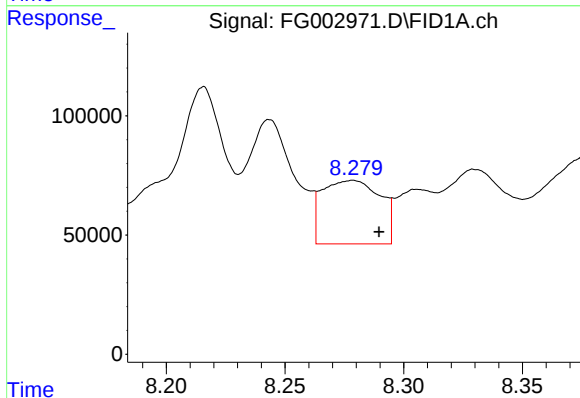


#4 N-TETRADECANE

R.T.: 8.278 min
Delta R.T.: -0.012 min
Response: 452286
Conc: 3.42 ug/ml

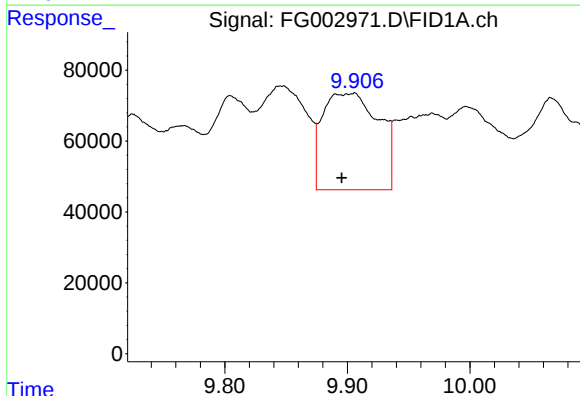


#5 N-HEXADECANE

R.T.: 9.904 min
Delta R.T.: 0.008 min
Response: 865307
Conc: 6.50 ug/ml

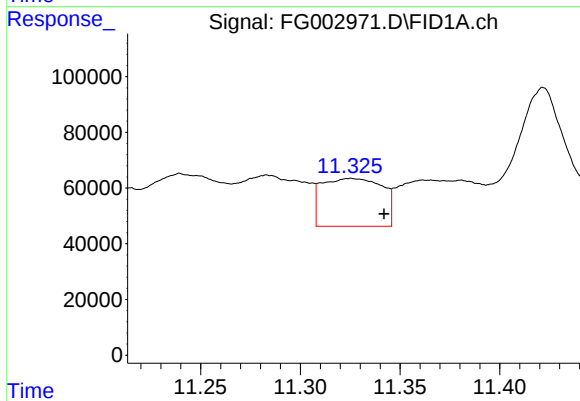


#6 N-OCTADECANE

R.T.: 11.326 min
Delta R.T.: -0.016 min
Response: 363468
Conc: 2.75 ug/ml

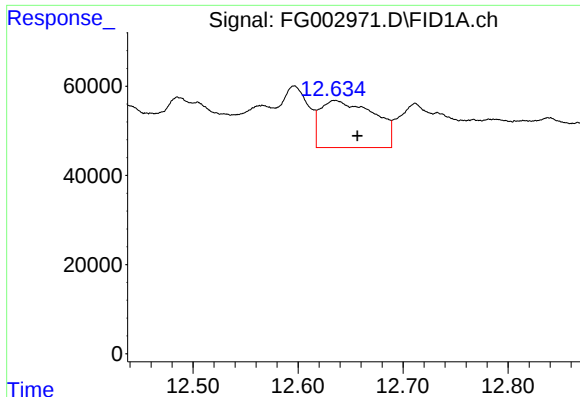


#7 N-EICOSANE

R.T.: 12.636 min
Delta R.T.: -0.021 min
Response: 376625
Conc: 2.91 ug/ml

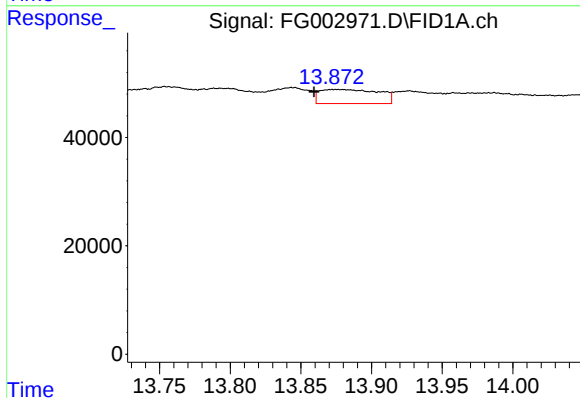


#8 N-DOCOSANE

R.T.: 13.875 min
Delta R.T.: 0.016 min
Response: 76435
Conc: 0.60 ug/ml

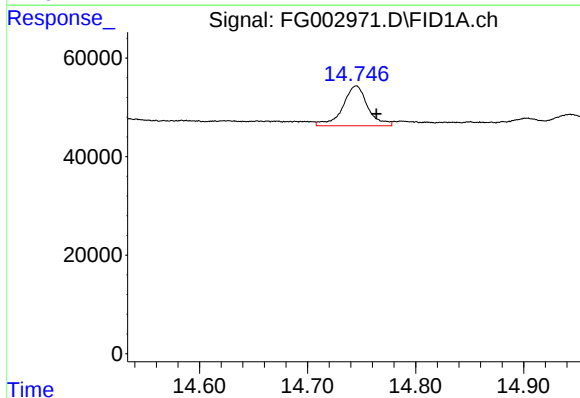


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.745 min
Delta R.T.: -0.019 min
Response: 130369
Conc: 1.19 ug/ml

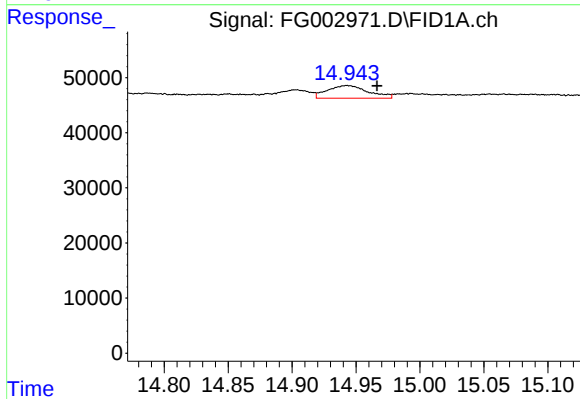


#10 N-TETRACOSANE

R.T.: 14.943 min
Delta R.T.: -0.023 min
Response: 51483
Conc: 0.41 ug/ml

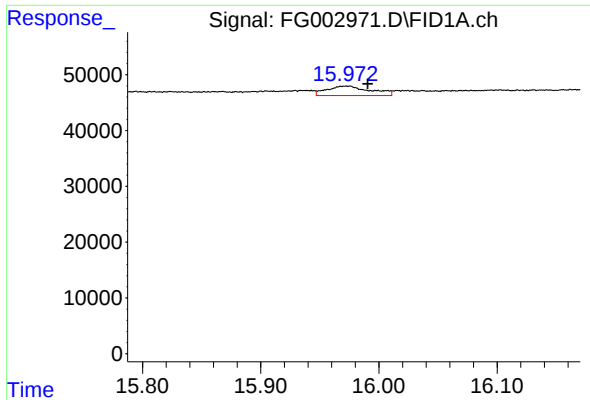

#11 N-HEXACOSANE

R.T.: 15.972 min
Delta R.T.: -0.018 min
Response: 44321
Conc: 0.36 ug/ml

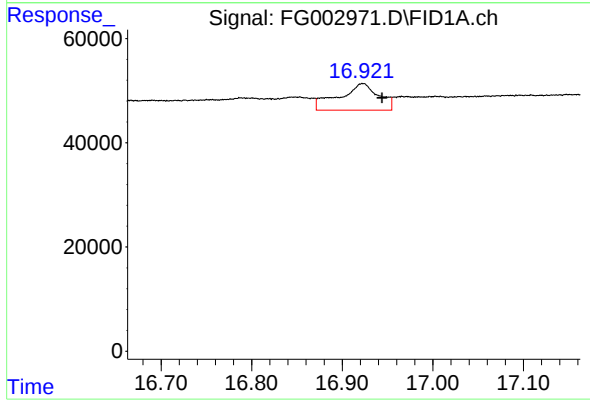

#12 N-OCTACOSANE

R.T.: 16.922 min
Delta R.T.: -0.022 min
Response: 155970
Conc: 1.28 ug/ml