

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111521\
 Data File : FG009071.D
 Signal(s) : FID1A.ch
 Acq On : 15 Nov 2021 15:03
 Operator : AJ\MA
 Sample : M4693-01 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 UT-COMP-01

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/16/2021
 Supervised By :mohammad ahmed 11/16/2021

Integration File: autoint1.e
 Quant Time: Nov 16 00:56:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
 Quant Title :
 QLast Update : Tue Nov 02 01:56:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.756	343170	2.973 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111521\
Data File : FG009071.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2021 15:03
Operator : AJ\MA
Sample : M4693-01 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
UT-COMP-01


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/16/2021
Supervised By :mohammad ahmed 11/16/2021

Integration File: autoint1.e
Quant Time: Nov 16 00:56:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

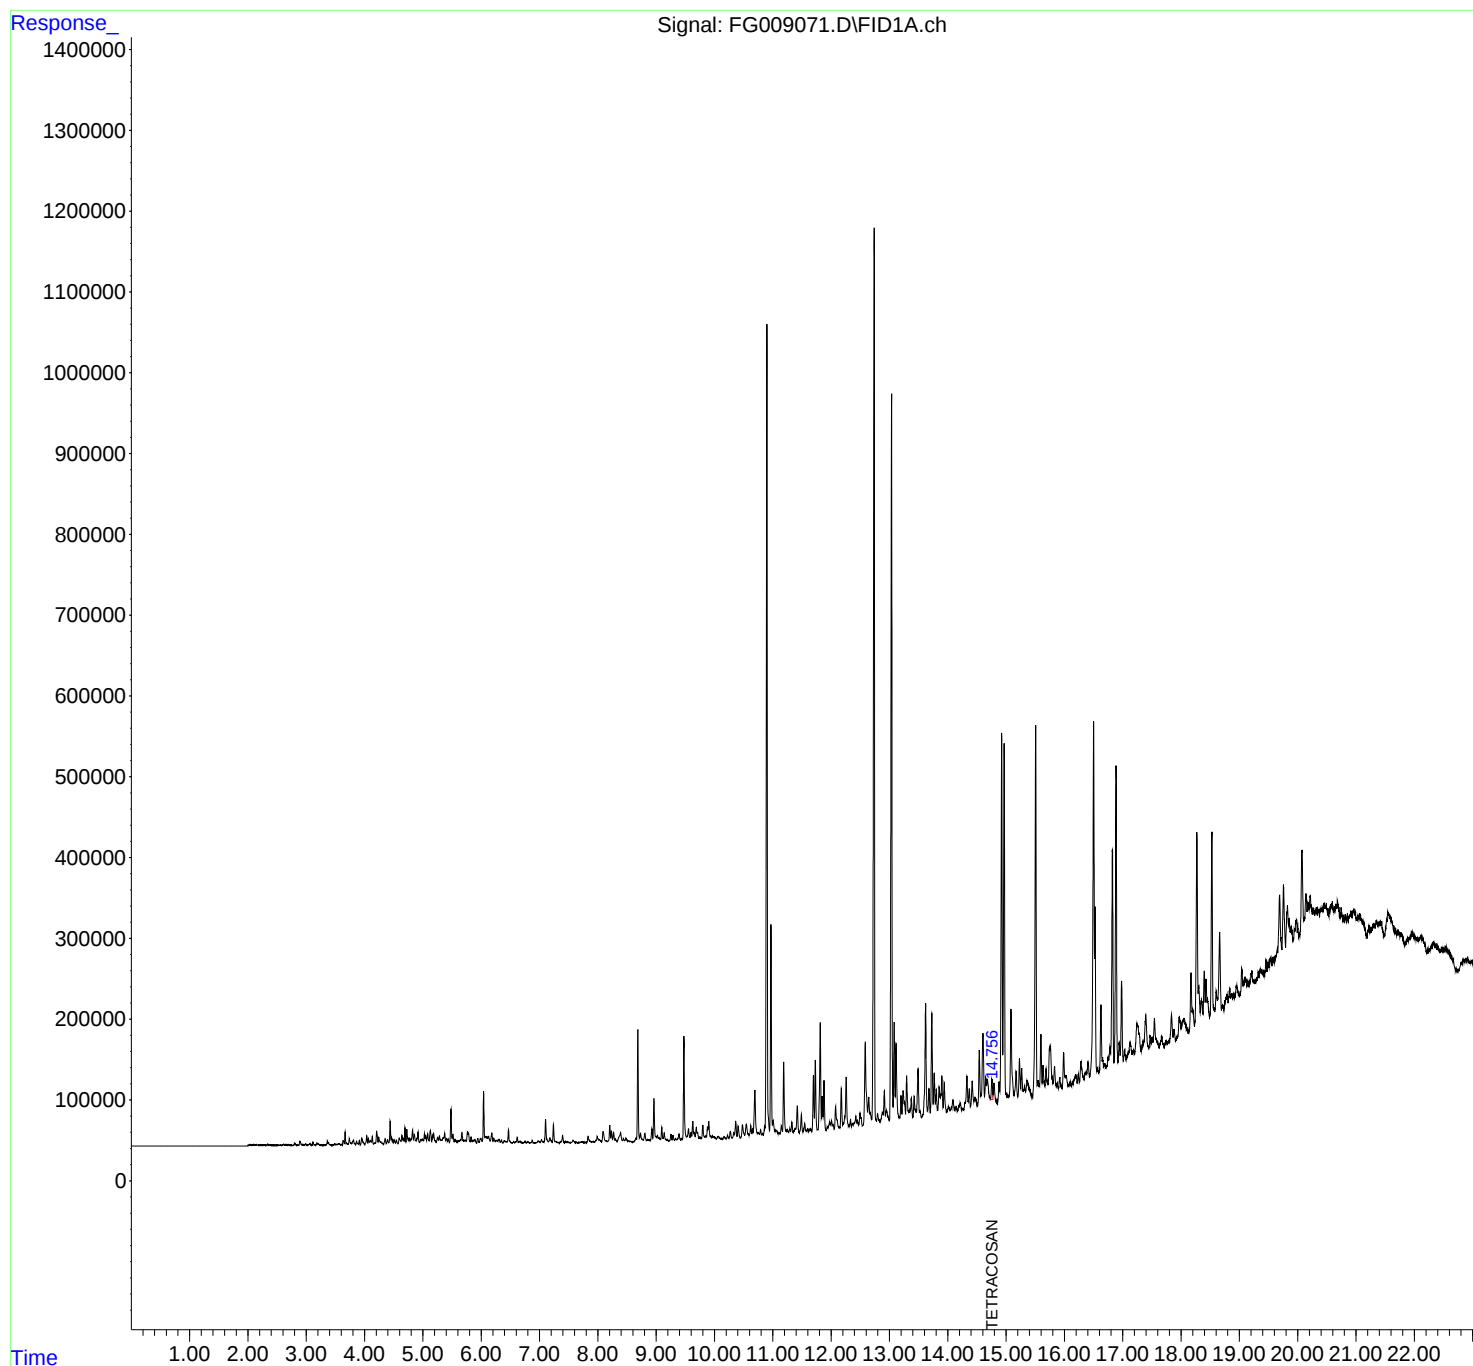

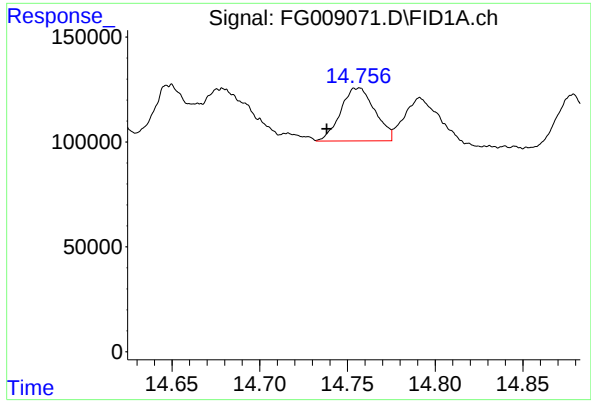

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.756 min
Delta R.T.: 0.018 min
Response: 343170
Conc: 2.97 ug/ml

Instrument :
FID_G
ClientSampleId :
UT-COMP-01

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/16/2021
Supervised By :mohammad ahmed 11/16/2021