

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111521\
Data File : FG009072.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2021 15:34
Operator : AJ\MA
Sample : M4693-03 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
UT-COMP-02

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/16/2021
Supervised By :mohammad ahmed 11/16/2021

Integration File: autoint1.e
Quant Time: Nov 16 00:57:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.754	204856	1.775 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111521\
Data File : FG009072.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2021 15:34
Operator : AJ\MA
Sample : M4693-03 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
UT-COMP-02


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/16/2021
Supervised By :mohammad ahmed 11/16/2021

Integration File: autoint1.e
Quant Time: Nov 16 00:57:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

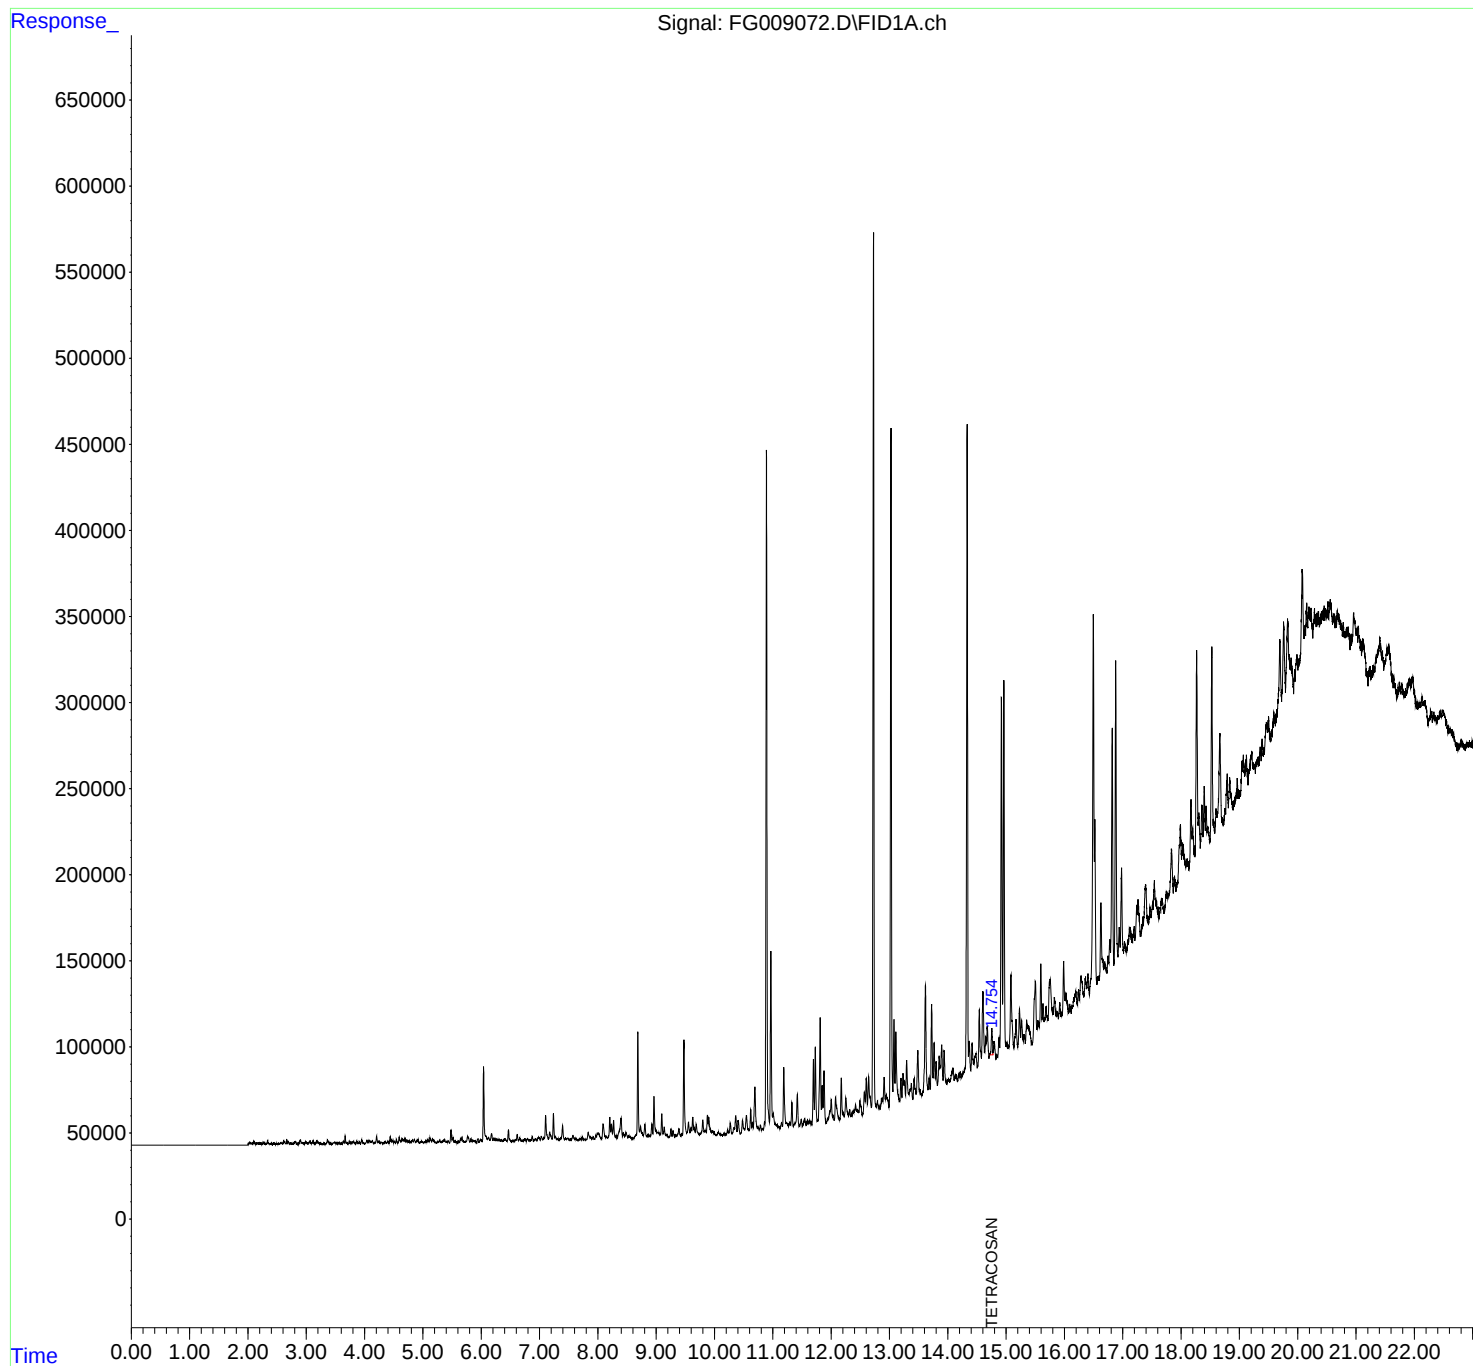

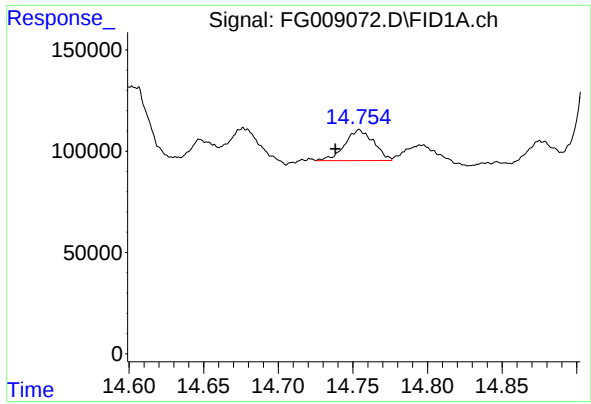

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.754 min
Delta R.T.: 0.016 min
Response: 204856
Conc: 1.77 ug/ml

Instrument :
FID_G
ClientSampleId :
UT-COMP-02

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/16/2021
Supervised By :mohammad ahmed 11/16/2021