

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111522\
Data File : FG011107.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2022 10:09
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 05:07:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
Quant Title :
QLast Update : Mon Nov 14 17:25:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.766	2931512	23.330 ug/ml
12)	N-OCTACOSANE	17.257	2855775	23.832 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111522\
Data File : FG011107.D
Signal(s) : FID1A.ch
Acq On : 15 Nov 2022 10:09
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 05:07:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
Quant Title :
QLast Update : Mon Nov 14 17:25:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

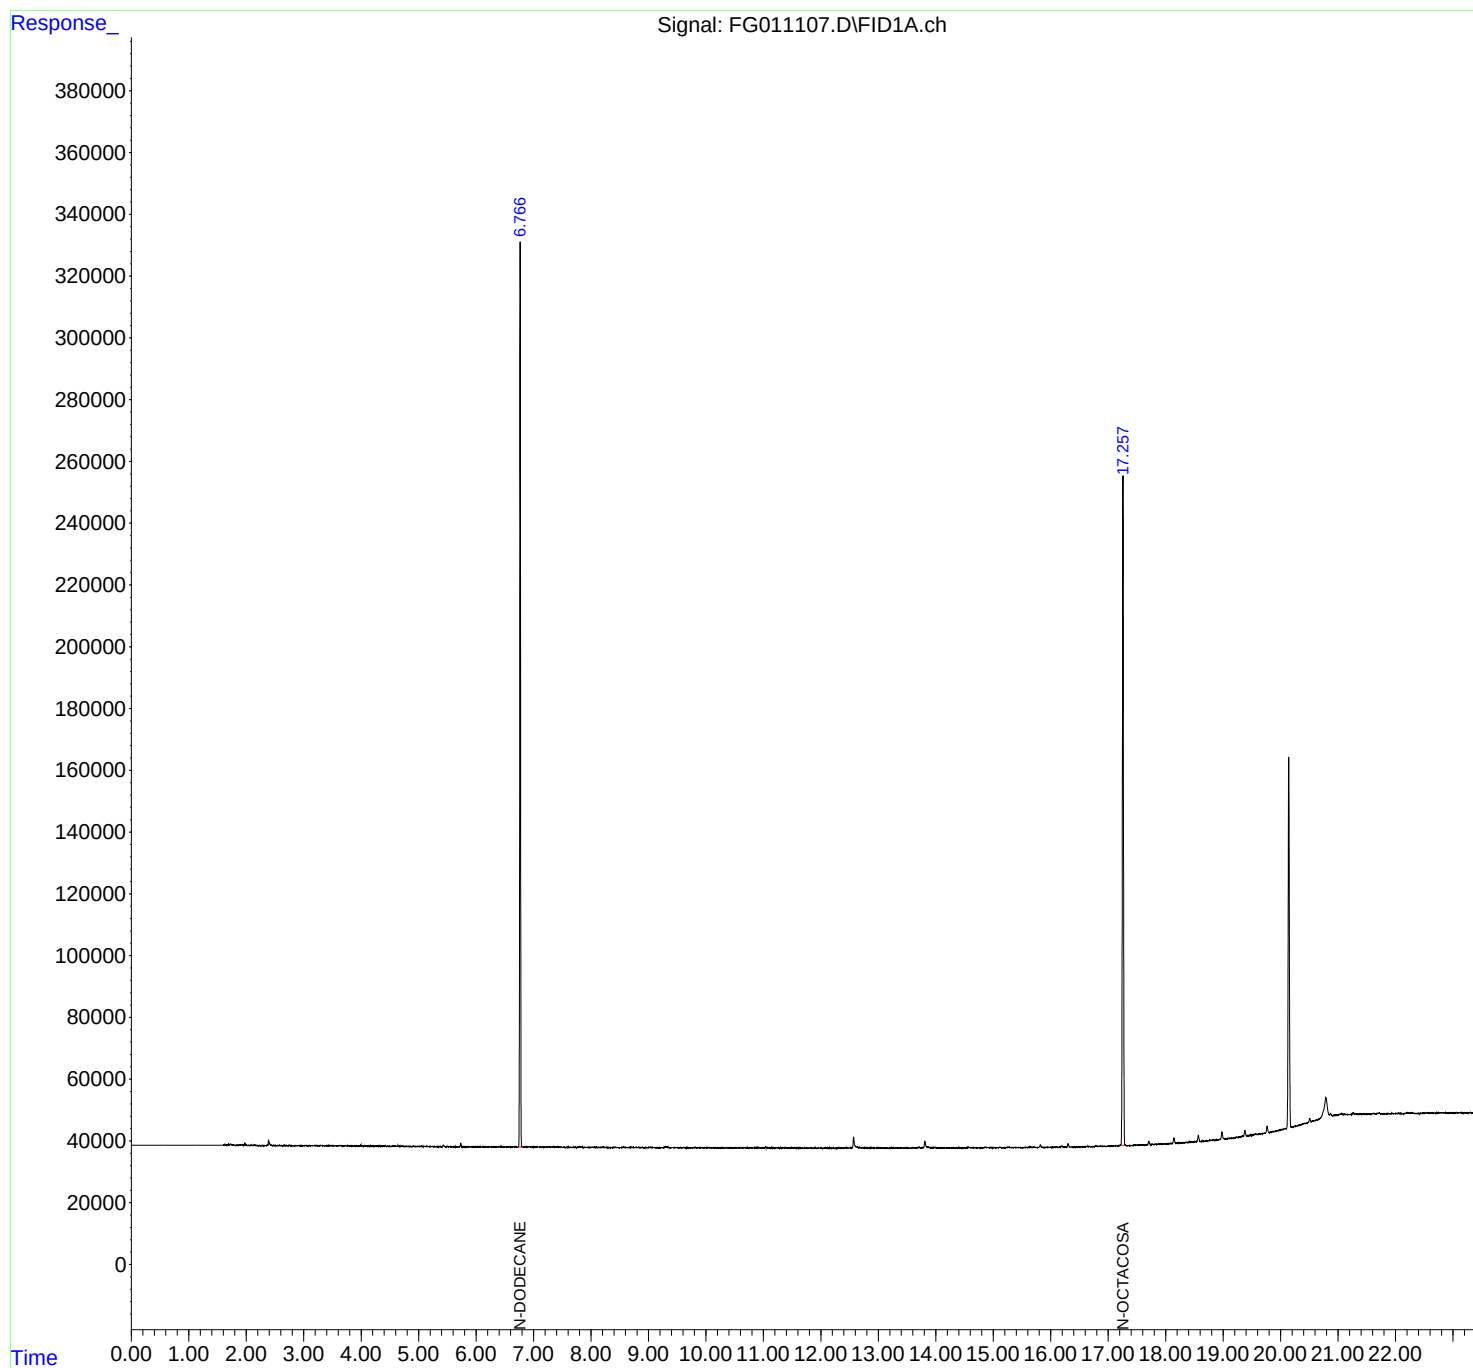


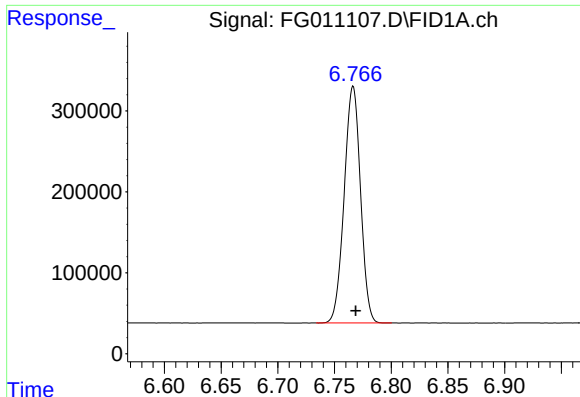

#3 N-DODECANE


R.T.: 6.766 min
Delta R.T.: -0.002 min
Response: 2931512
Conc: 23.33 ug/ml

Instrument :
FID_G
ClientSampleId :

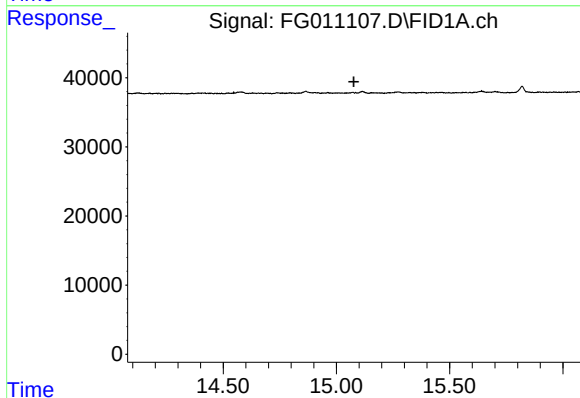

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.077 min
Response: 0
Conc: N.D.

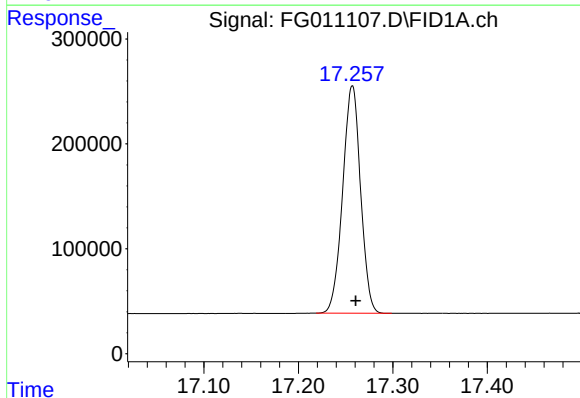

#12 N-OCTACOSANE

R.T.: 17.257 min
Delta R.T.: -0.003 min
Response: 2855775
Conc: 23.83 ug/ml