

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111618\
Data File : FG003002.D
Signal(s) : FID1A.ch
Acq On : 16 Nov 2018 22:24
Operator : AJ\SJ
Sample : J5950-02 50X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 16 23:57:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.500	199476	1.564 ug/ml
3) N-DODECANE	6.503	316007	2.424 ug/ml
4) N-TETRADECANE	8.302	205696	1.556 ug/ml
5) N-HEXADECANE	9.891	384796	2.890 ug/ml
6) N-OCTADECANE	11.278f	165956	1.255 ug/ml
7) N-EICOSANE	12.591f	93763	0.723 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111618\
Data File : FG003002.D
Signal(s) : FID1A.ch
Acq On : 16 Nov 2018 22:24
Operator : AJ\SJ
Sample : J5950-02 50X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 16 23:57:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

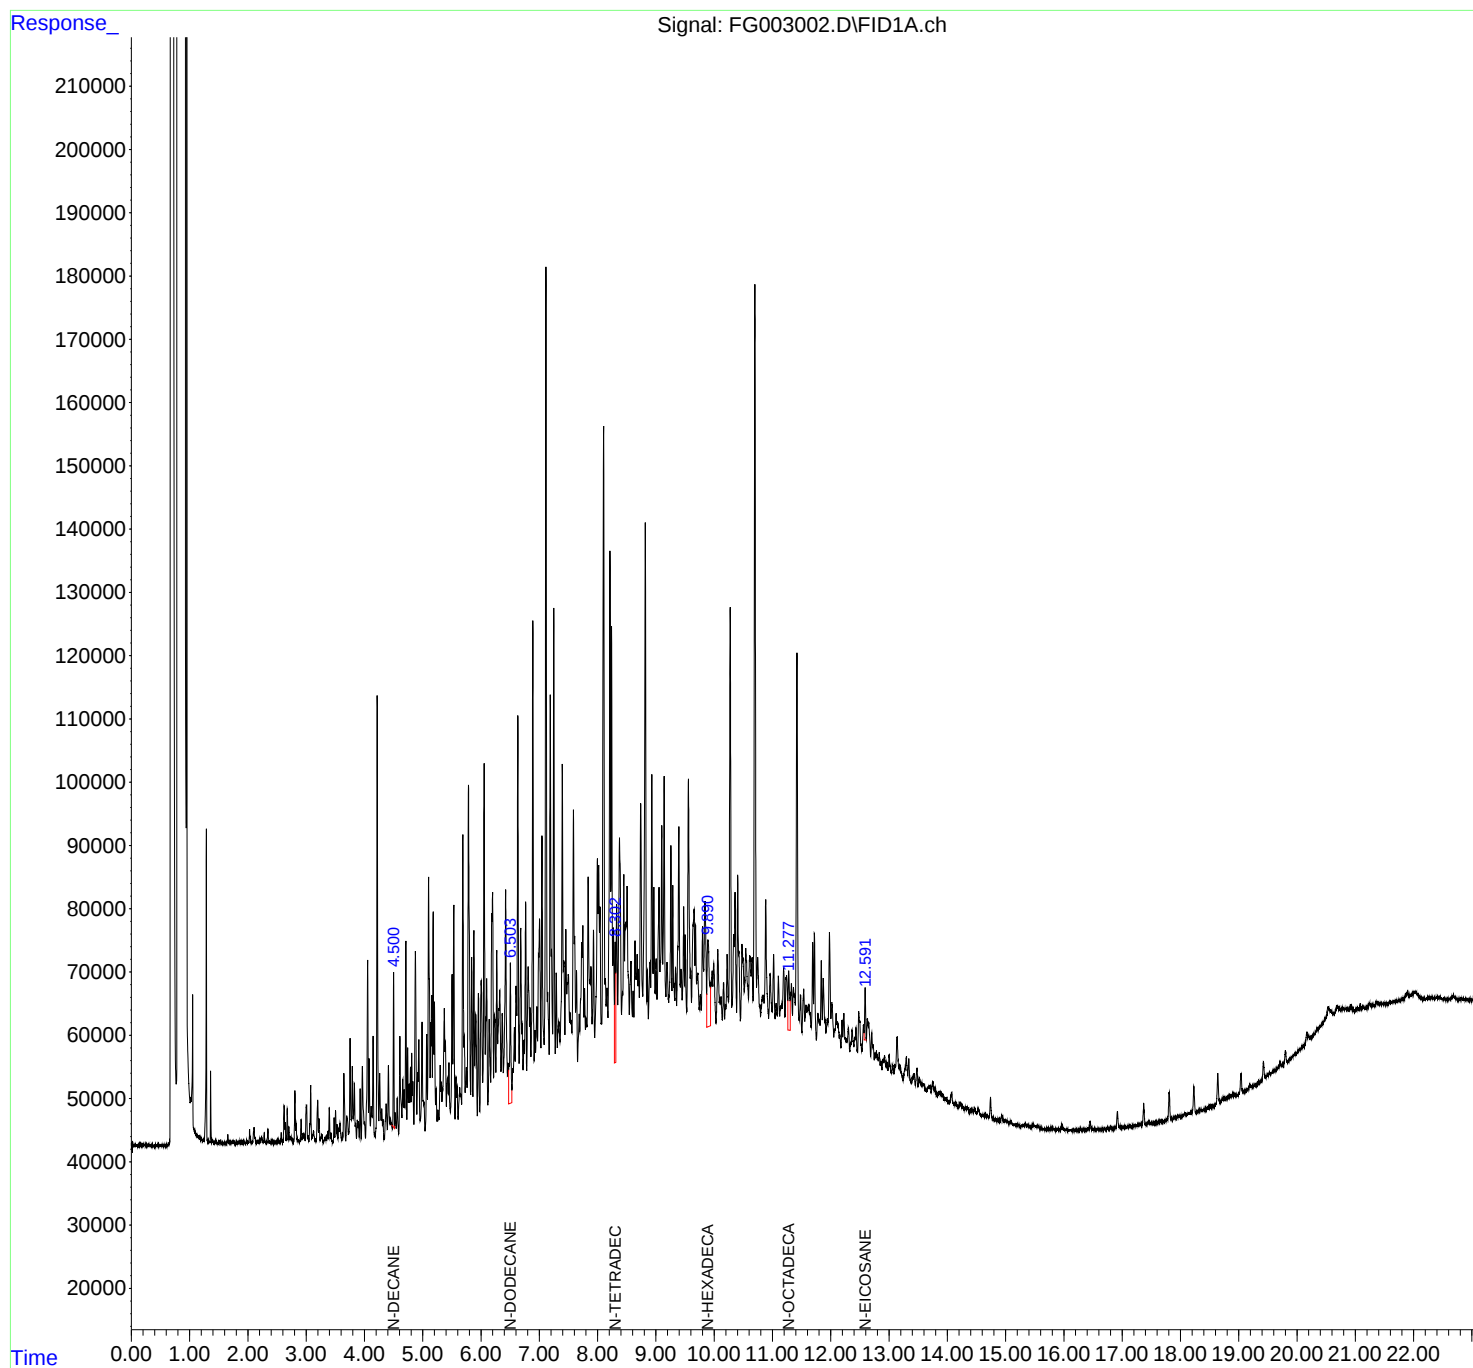

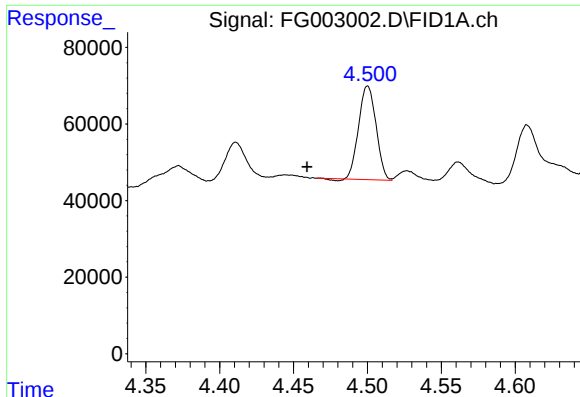


#2 N-DECANE

R.T.: 4.500 min
Delta R.T.: 0.041 min
Response: 199476
Conc: 1.56 ug/ml

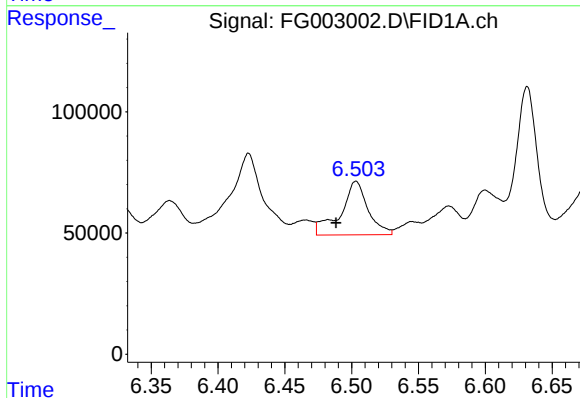


#3 N-DODECANE

R.T.: 6.503 min
Delta R.T.: 0.015 min
Response: 316007
Conc: 2.42 ug/ml

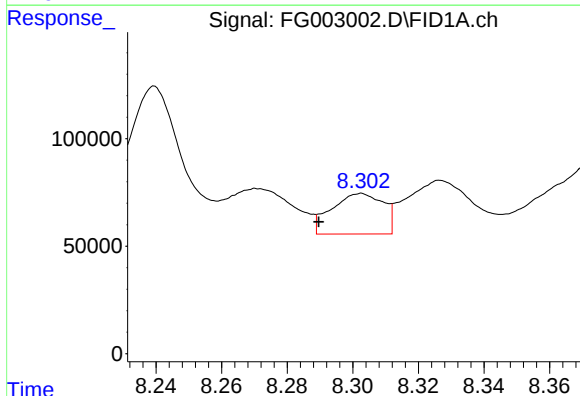


#4 N-TETRADECANE

R.T.: 8.302 min
Delta R.T.: 0.013 min
Response: 205696
Conc: 1.56 ug/ml

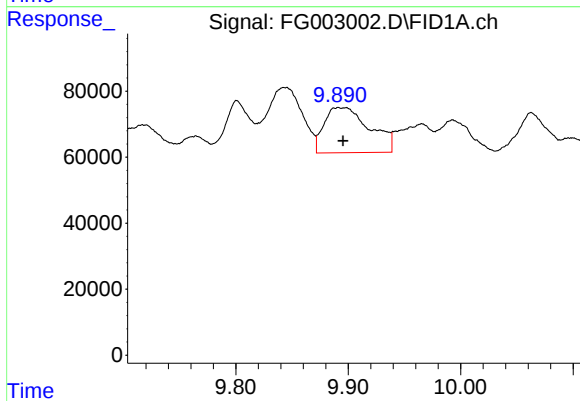


#5 N-HEXADECANE

R.T.: 9.891 min
Delta R.T.: -0.004 min
Response: 384796
Conc: 2.89 ug/ml

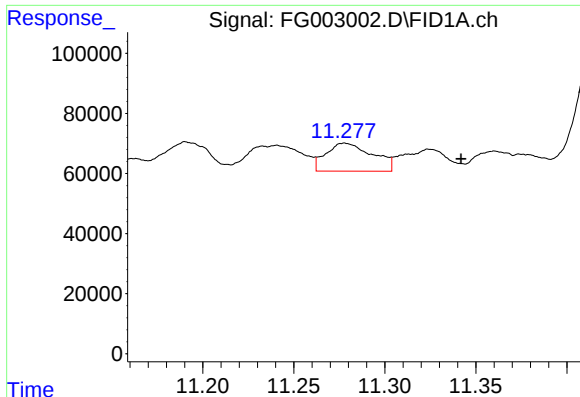


#6 N-OCTADECANE

R.T.: 11.278 min
Delta R.T.: -0.064 min
Response: 165956
Conc: 1.25 ug/ml

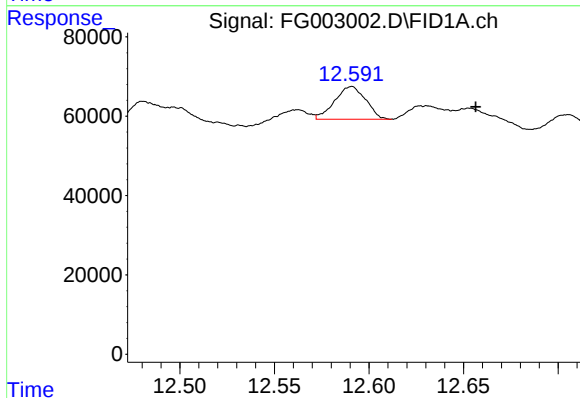

#7 N-EICOSANE

R.T.: 12.591 min
Delta R.T.: -0.066 min
Response: 93763
Conc: 0.72 ug/ml

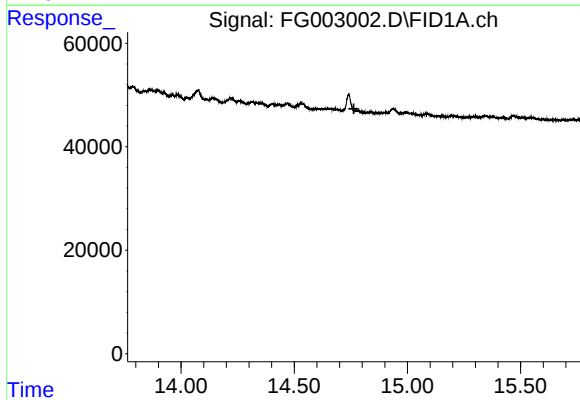

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.764 min
Response: 0
Conc: N.D.