

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111723\
Data File : FG013198.D
Signal(s) : FID1A.ch
Acq On : 17 Nov 2023 15:16
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 17 21:31:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111023.M
Quant Title :
QLast Update : Fri Nov 10 12:13:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.081	1716729	16.748 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.268	71870	0.634 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111723\
Data File : FG013198.D
Signal(s) : FID1A.ch
Acq On : 17 Nov 2023 15:16
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 17 21:31:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111023.M
Quant Title :
QLast Update : Fri Nov 10 12:13:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

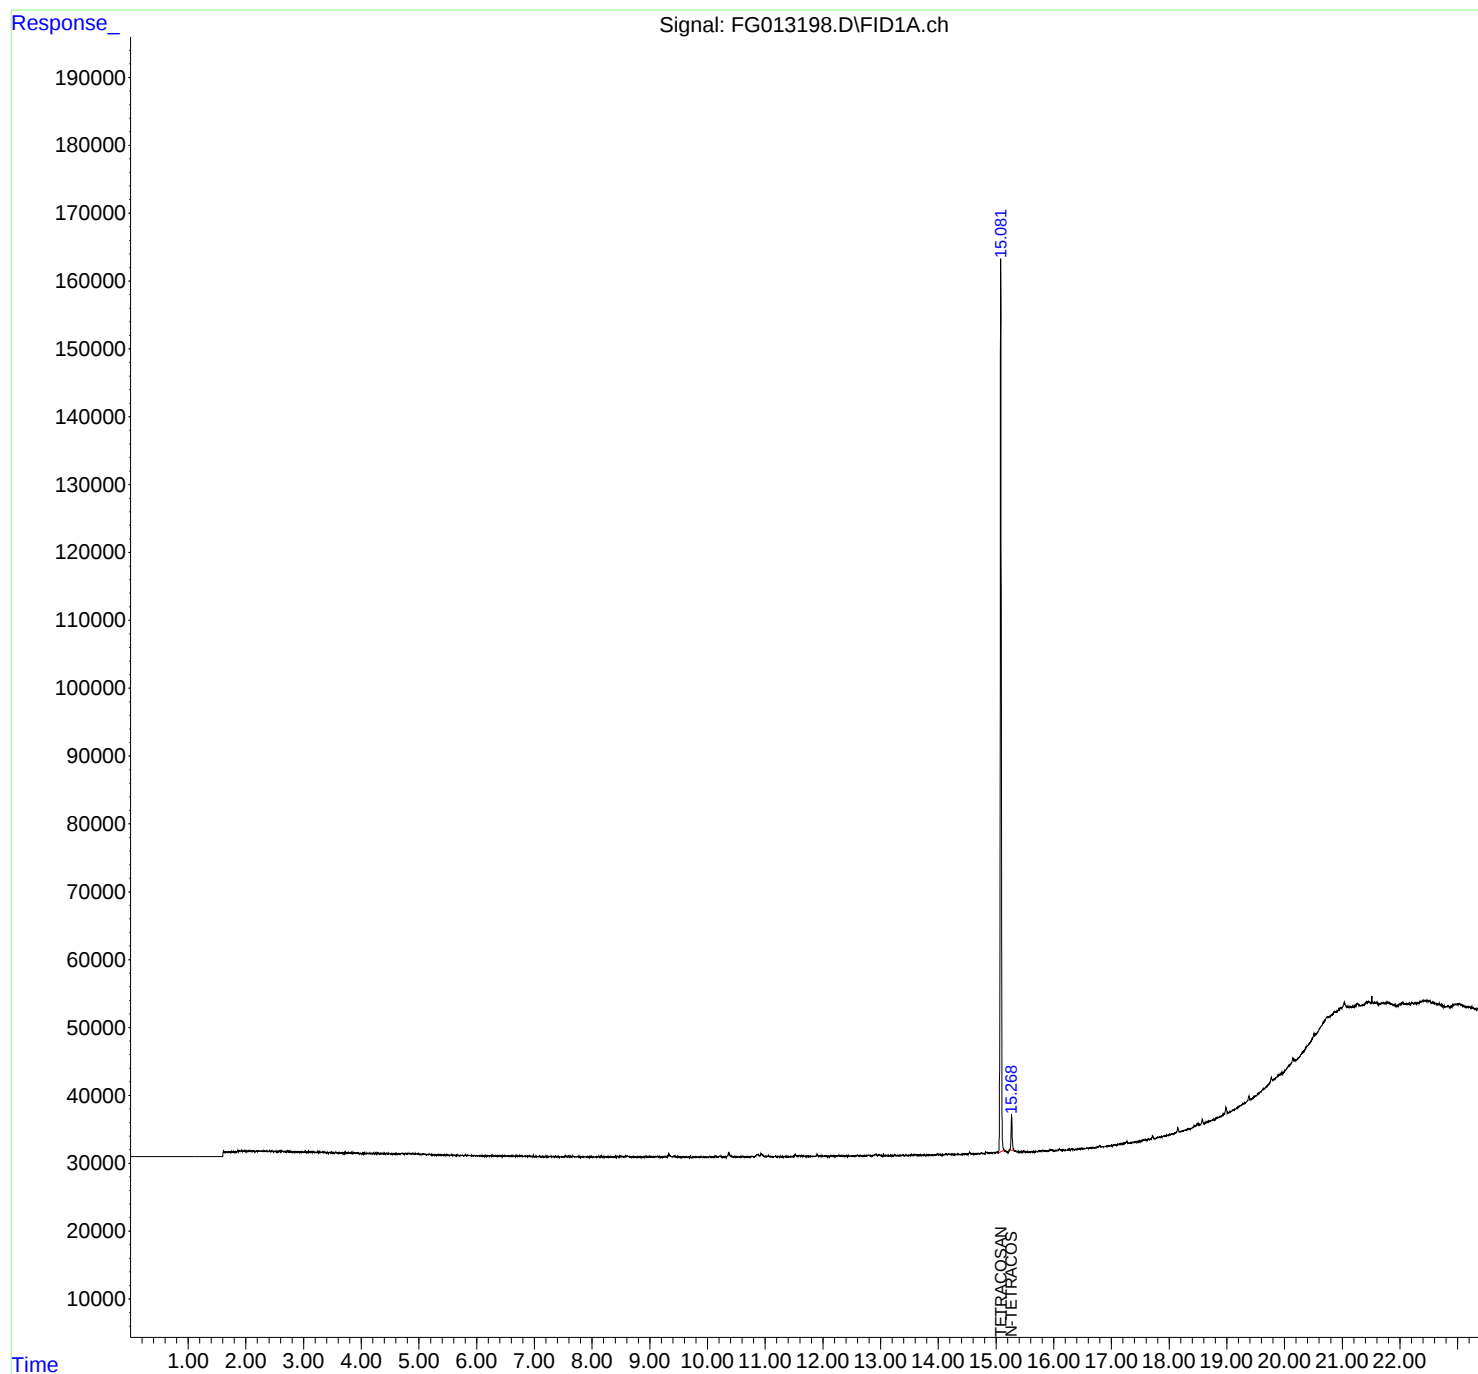


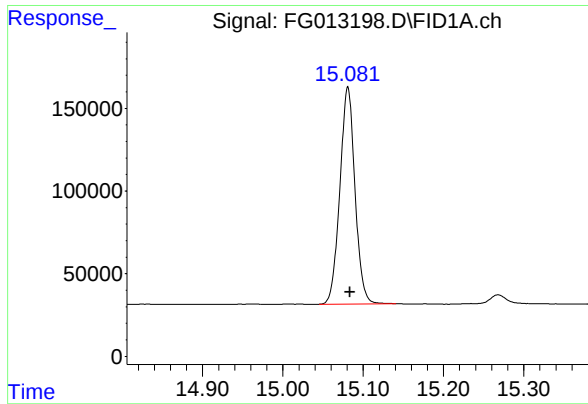

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.081 min
Delta R.T.: -0.003 min
Response: 1716729
Conc: 16.75 ug/ml

Instrument :
FID_G
ClientSampleId :

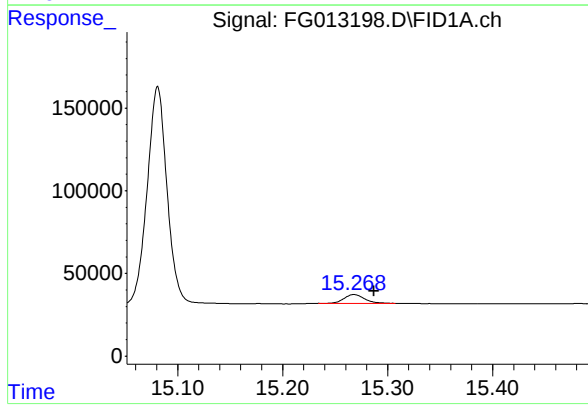

#10 N-TETRACOSANE

R.T.: 15.268 min
Delta R.T.: -0.019 min
Response: 71870
Conc: 0.63 ug/ml