

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111723\
Data File : FG013194.D
Signal(s) : FID1A.ch
Acq On : 17 Nov 2023 13:20
Operator : YP\AJ
Sample : 05320-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MW-03

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :Ankita Jodhani 11/21/2023

Integration File: autoint1.e
Quant Time: Nov 17 21:31:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111023.M
Quant Title :
QLast Update : Fri Nov 10 12:13:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.095	84535	0.825 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111723\
Data File : FG013194.D
Signal(s) : FID1A.ch
Acq On : 17 Nov 2023 13:20
Operator : YP\AJ
Sample : 05320-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
MW-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :Ankita Jodhani 11/21/2023

Integration File: autoint1.e
Quant Time: Nov 17 21:31:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111023.M
Quant Title :
QLast Update : Fri Nov 10 12:13:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

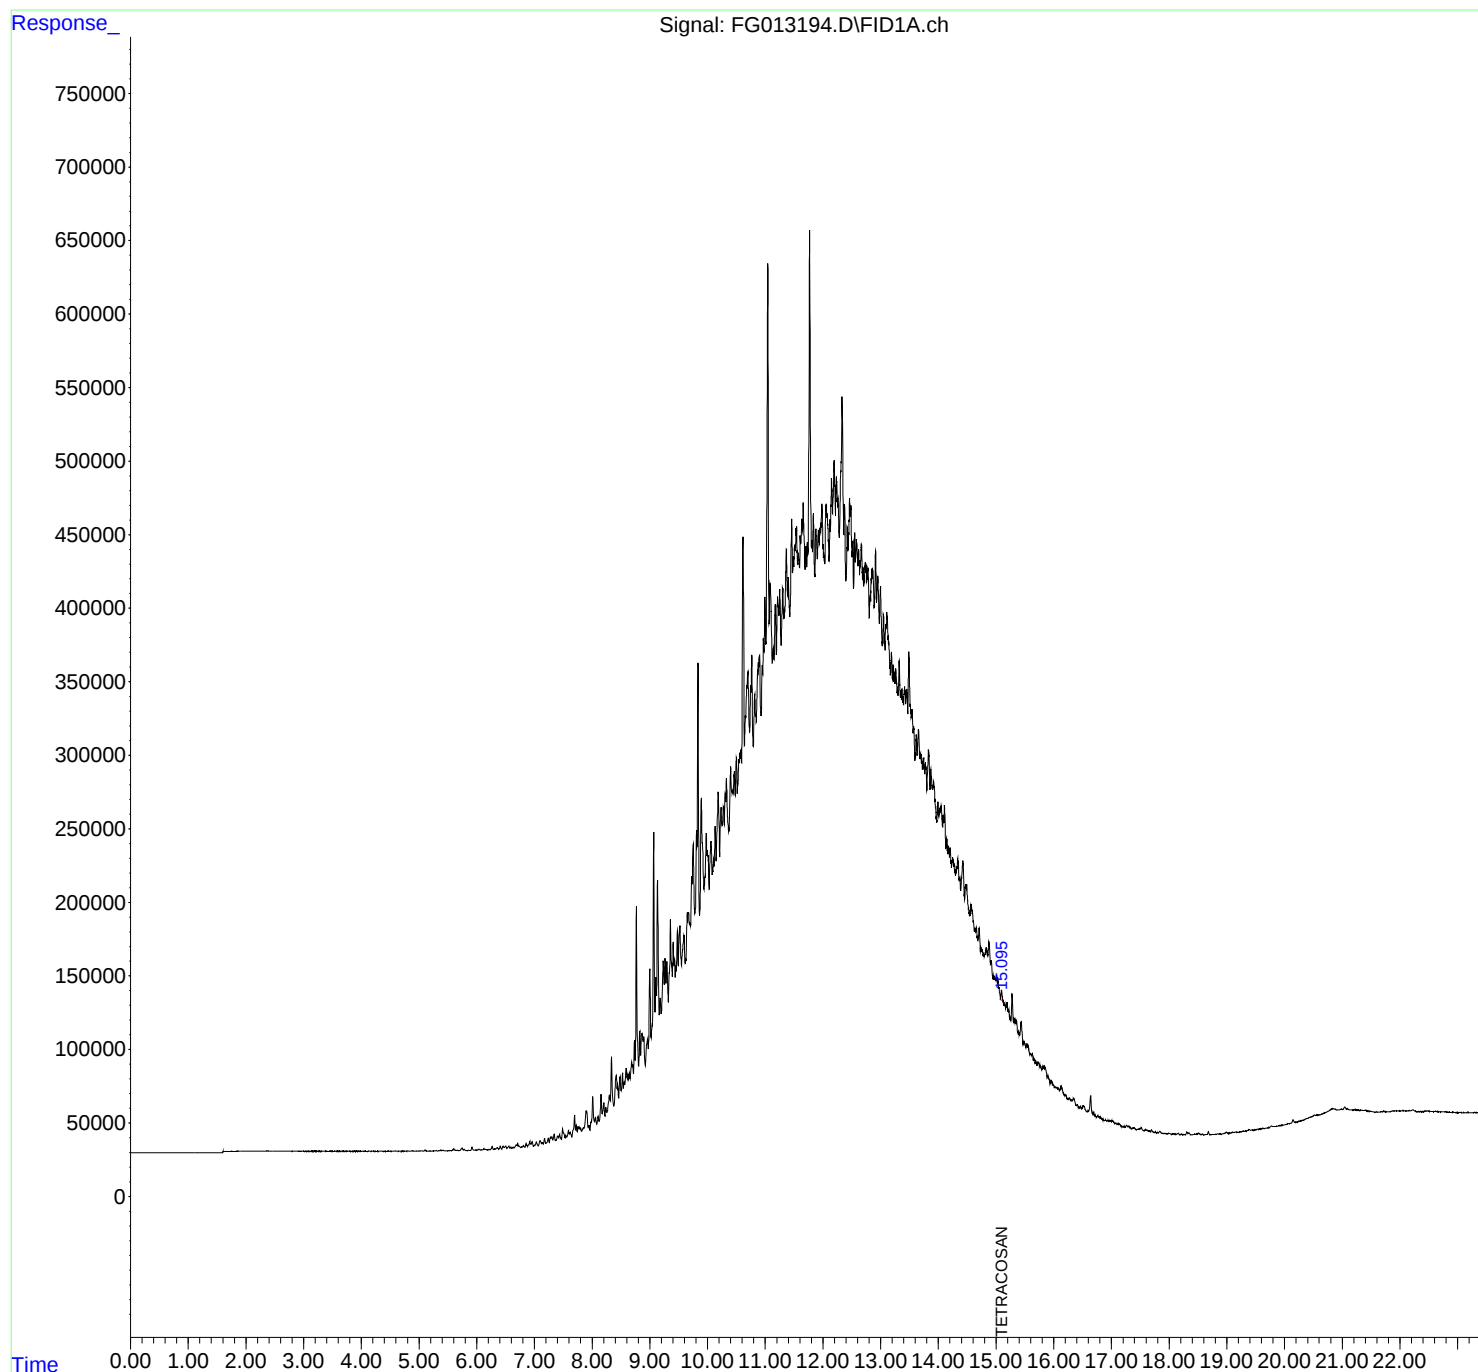

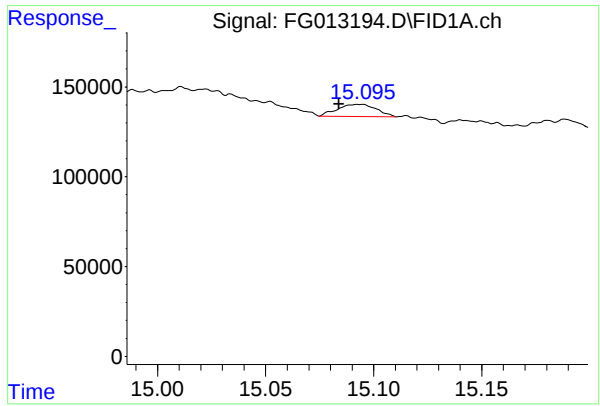

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.095 min
Delta R.T.: 0.011 min
Response: 84535
Conc: 0.82 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-03

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2023
Supervised By :Ankita Jodhani 11/21/2023