

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111820\
Data File : FG007365.D
Signal(s) : FID1A.ch
Acq On : 18 Nov 2020 14:51
Operator : DD\AJ
Sample : L4784-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-02-20201117

Integration File: autoint1.e
Quant Time: Nov 19 00:30:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.733	2303052	18.720 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111820\
Data File : FG007365.D
Signal(s) : FID1A.ch
Acq On : 18 Nov 2020 14:51
Operator : DD\AJ
Sample : L4784-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-02-20201117

Integration File: autoint1.e
Quant Time: Nov 19 00:30:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

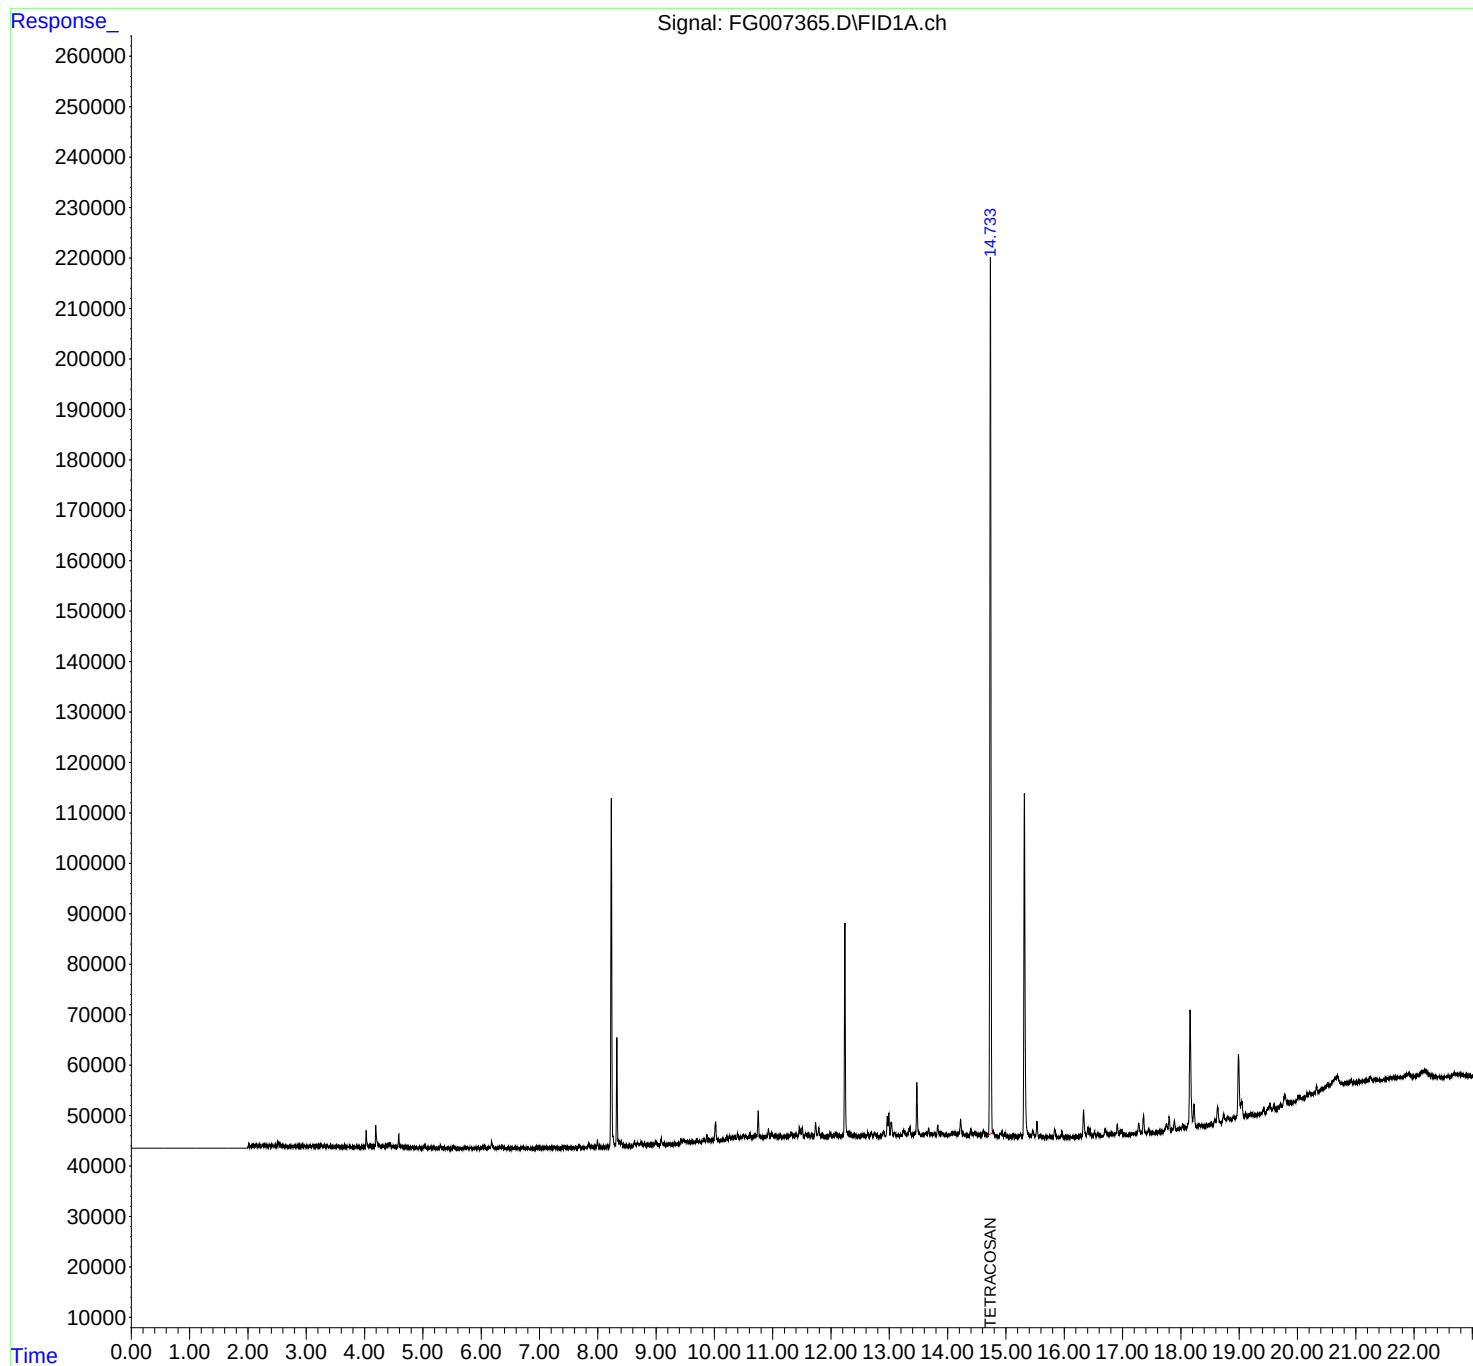

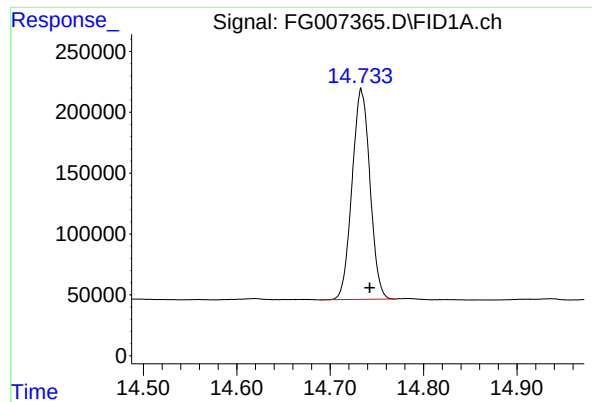

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.733 min
Delta R.T.: -0.009 min
Response: 2303052
Conc: 18.72 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-02-20201117