

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111824\
 Data File : FG014859.D
 Signal(s) : FID1A.ch
 Acq On : 18 Nov 2024 19:05
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Nov 19 01:32:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111324.M
 Quant Title :
 QLast Update : Wed Nov 13 13:49:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.044	5539607	49.386 ug/ml
Target Compounds			
2) N-DECANE	4.569	6568019	52.013 ug/ml
3) N-DODECANE	6.741	6644877	51.162 ug/ml
4) N-TETRADECANE	8.573	6630306	52.611 ug/ml
5) N-HEXADECANE	10.184	6583671	51.620 ug/ml
6) N-OCTADECANE	11.630	6628925	50.623 ug/ml
7) N-EICOSANE	12.942	6618423	51.978 ug/ml
8) N-DOCOSANE	14.144	6326510	50.648 ug/ml
10) N-TETRACOSANE	15.249	6212385	50.290 ug/ml
11) N-HEXACOSANE	16.270	6078614	50.527 ug/ml
12) N-OCTACOSANE	17.221	5958201	50.679 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111824\
Data File : FG014859.D
Signal(s) : FID1A.ch
Acq On : 18 Nov 2024 19:05
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Nov 19 01:32:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111324.M
Quant Title :
QLast Update : Wed Nov 13 13:49:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

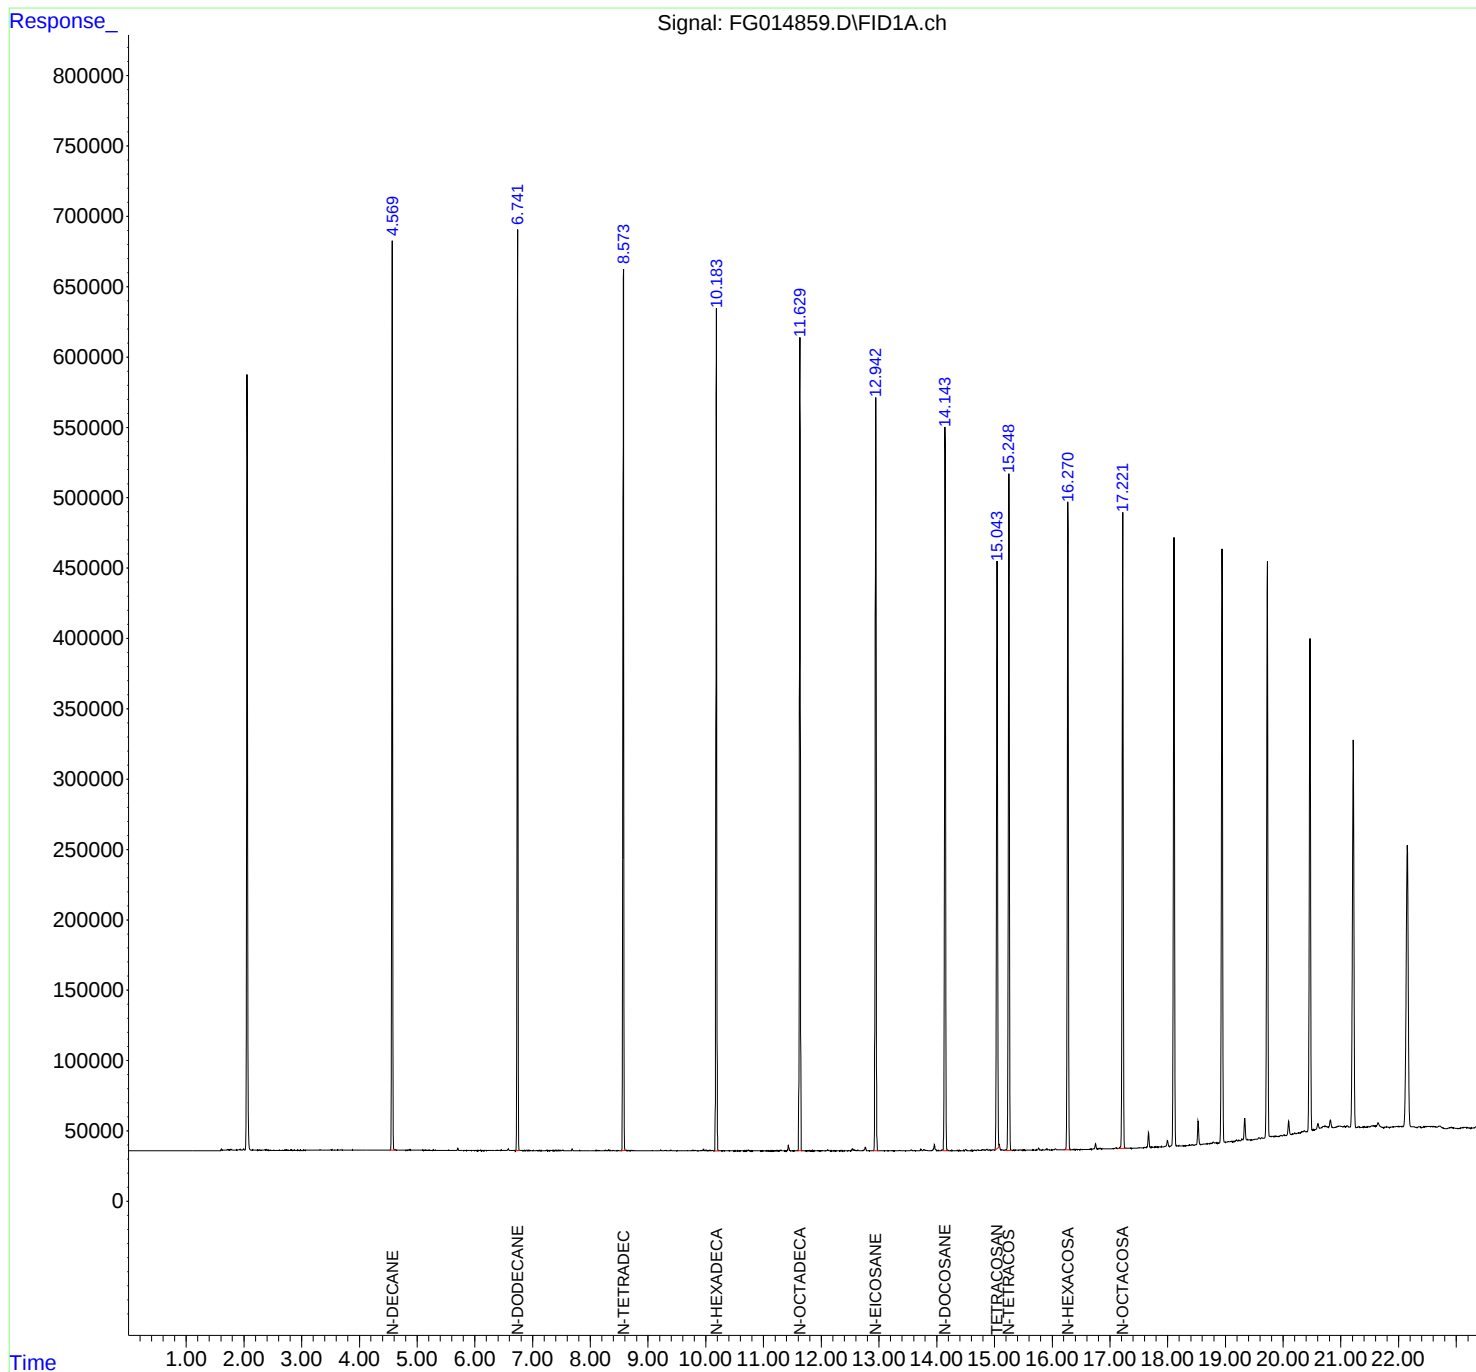


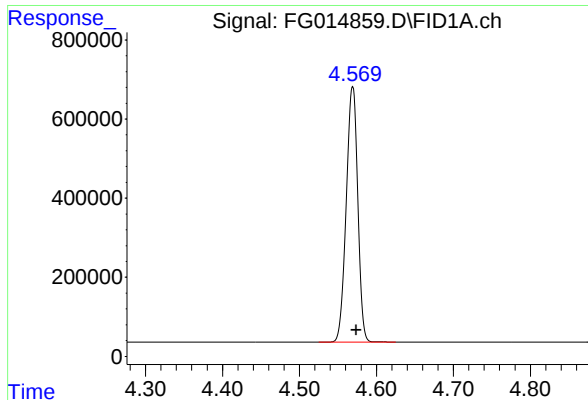

#2 N-DECANE


R.T.: 4.569 min
Delta R.T.: -0.005 min
Response: 6568019
Conc: 52.01 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

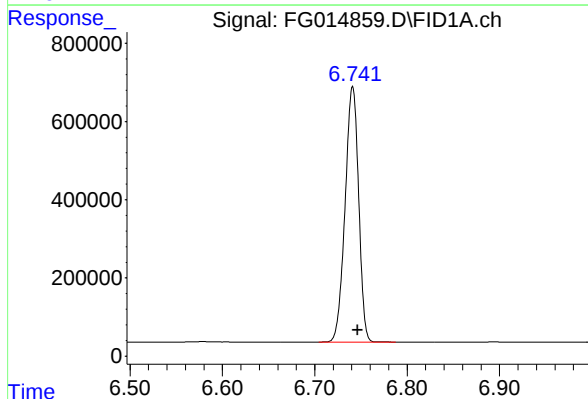


#3 N-DODECANE

R.T.: 6.741 min
Delta R.T.: -0.006 min
Response: 6644877
Conc: 51.16 ug/ml

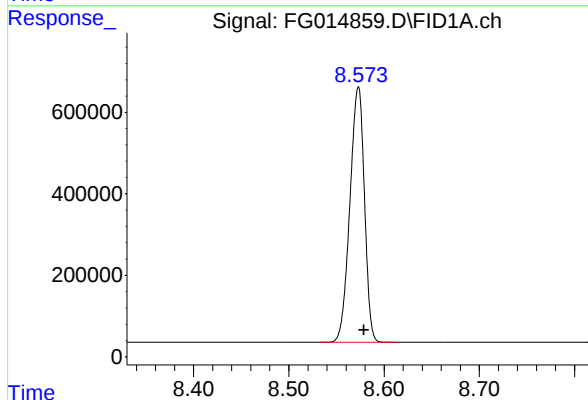


#4 N-TETRADECANE

R.T.: 8.573 min
Delta R.T.: -0.006 min
Response: 6630306
Conc: 52.61 ug/ml

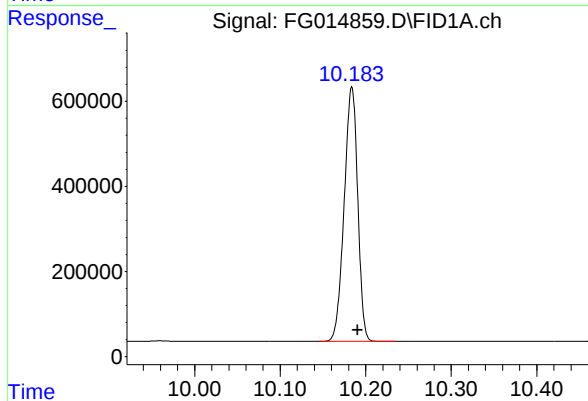

#5 N-HEXADECANE


R.T.: 10.184 min
Delta R.T.: -0.007 min
Response: 6583671
Conc: 51.62 ug/ml

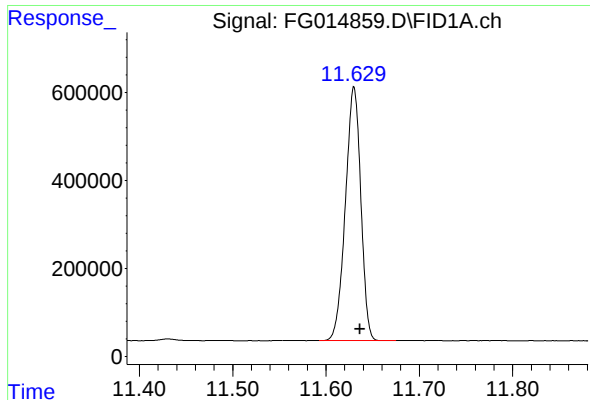

#6 N-OCTADECANE


R.T.: 11.630 min
Delta R.T.: -0.007 min
Response: 6628925
Conc: 50.62 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

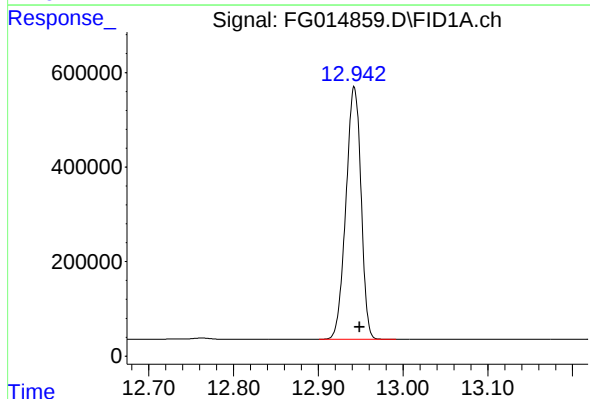


#7 N-EICOSANE

R.T.: 12.942 min
Delta R.T.: -0.006 min
Response: 6618423
Conc: 51.98 ug/ml

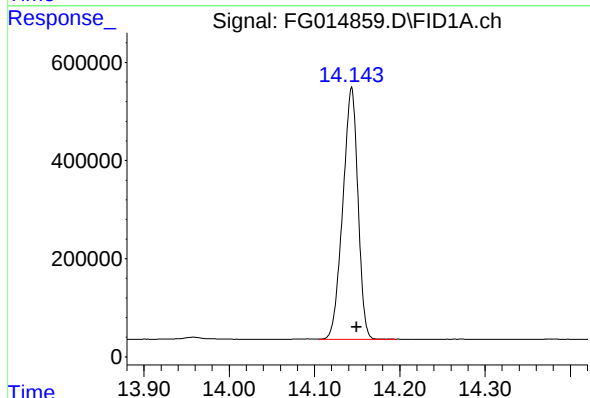


#8 N-DOCOSANE

R.T.: 14.144 min
Delta R.T.: -0.006 min
Response: 6326510
Conc: 50.65 ug/ml

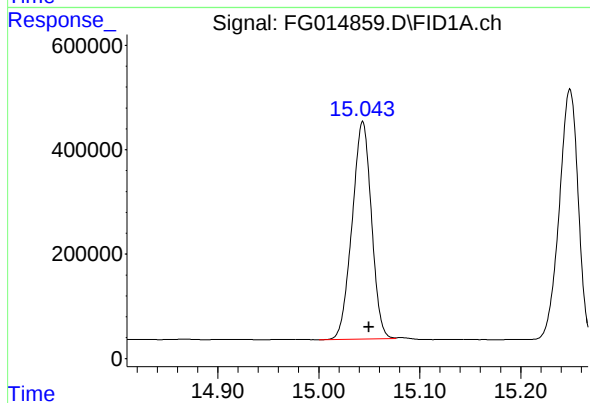

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.044 min
Delta R.T.: -0.006 min
Response: 5539607
Conc: 49.39 ug/ml

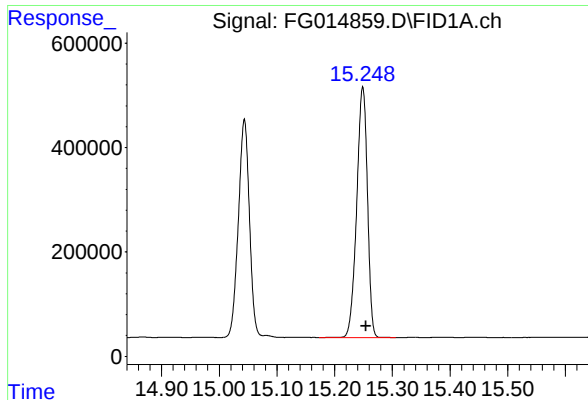

#10 N-TETRACOSANE


R.T.: 15.249 min
Delta R.T.: -0.006 min
Response: 6212385
Conc: 50.29 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

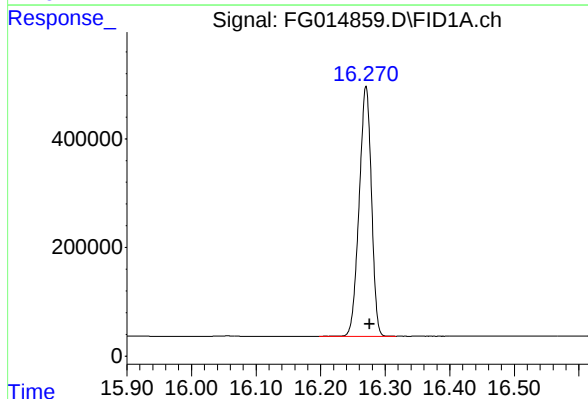

#11 N-HEXACOSANE

R.T.: 16.270 min
Delta R.T.: -0.006 min
Response: 6078614
Conc: 50.53 ug/ml

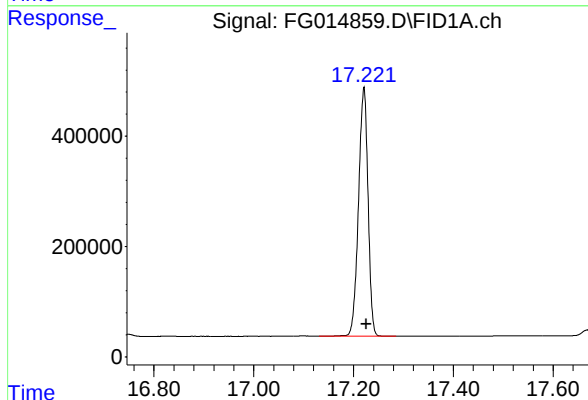

#12 N-OCTACOSANE

R.T.: 17.221 min
Delta R.T.: -0.005 min
Response: 5958201
Conc: 50.68 ug/ml