

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111924AL\
 Data File : FG014860.D
 Signal(s) : FID1A.ch
 Acq On : 19 Nov 2024 08:39
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 20 00:35:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 111424.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 14 16:33:02 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.440f	91952	0.827 ug/ml
Spiked Amount 50.000		Recovery =	1.65%
Target Compounds			
11) T n-Heneicosane (C21)	13.549	110323	0.850 ug/ml
14) T n-Tetracosane (C24)	15.243	97871	0.783 ug/ml
16) T n-Octacosane (C28)	17.173	65040	0.542 ug/ml
17) T n-Tricontane (C30)	18.163f	111005	0.885 ug/ml
18) T n-Dotriacontane (C32)	18.967	114677	0.921 ug/ml
20) T n-Hexatriacontane (C36)	20.464	66352	0.717 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111924AL\
Data File : FG014860.D
Signal(s) : FID1A.ch
Acq On : 19 Nov 2024 08:39
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 20 00:35:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 111424.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 16:33:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

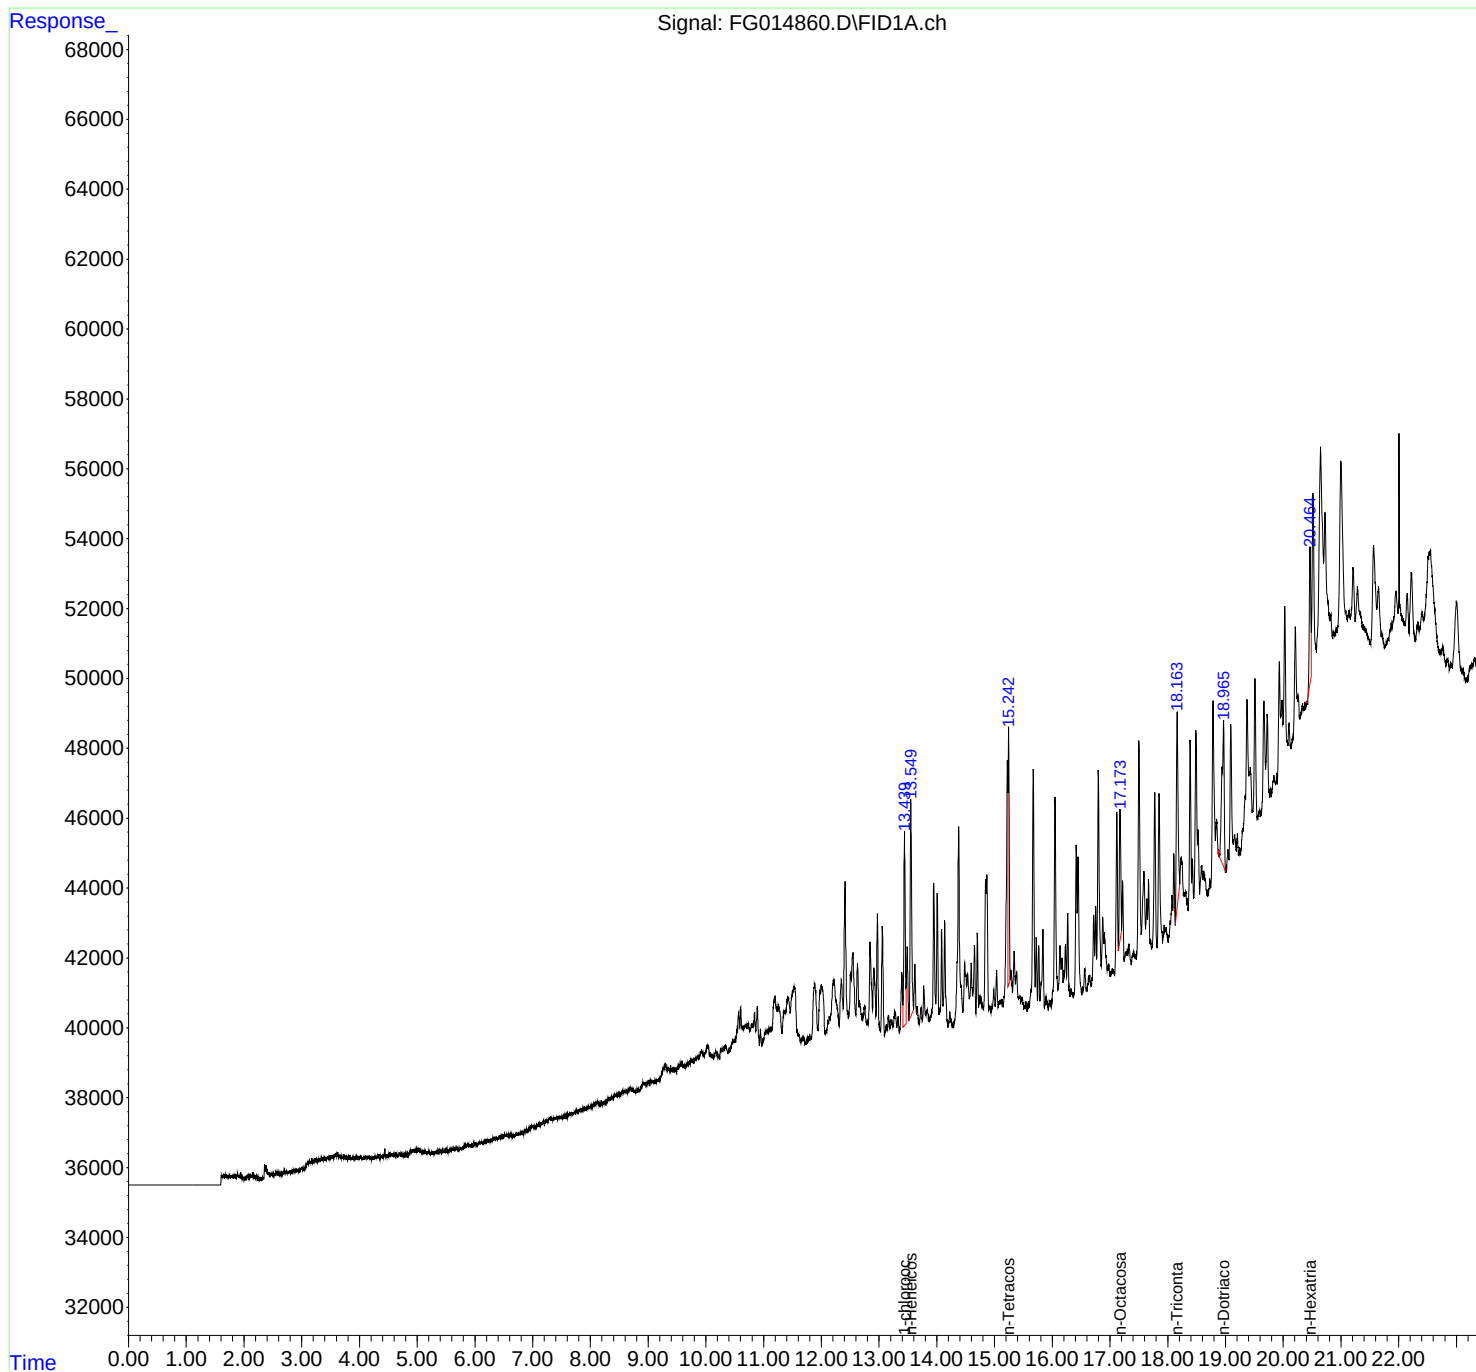


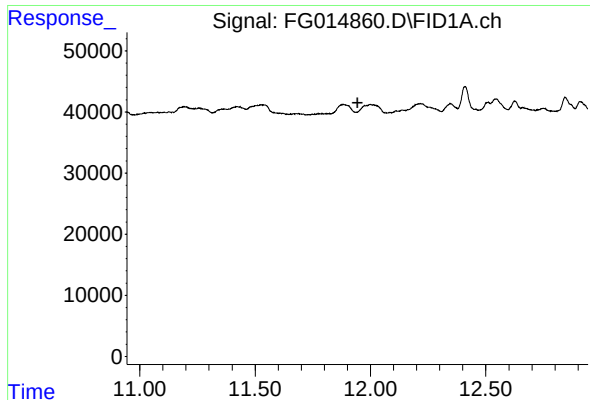

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.944 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

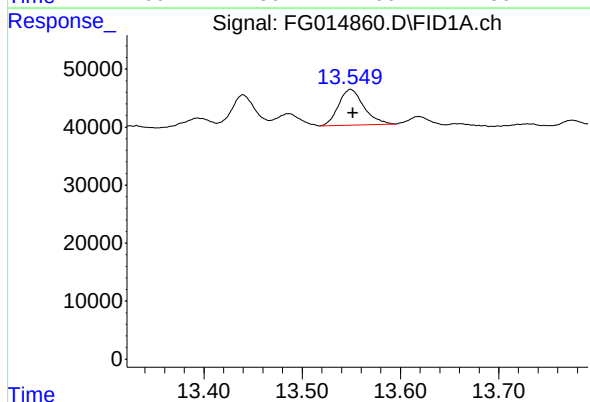


#11 n-Heneicosane (C21)

R.T.: 13.549 min
Delta R.T.: -0.002 min
Response: 110323
Conc: 0.85 ug/ml

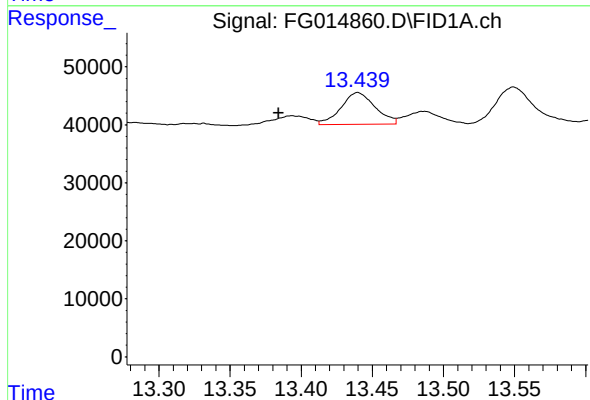


#12 1-chlorooctadecane (SURR)

R.T.: 13.440 min
Delta R.T.: 0.055 min
Response: 91952
Conc: 0.83 ug/ml

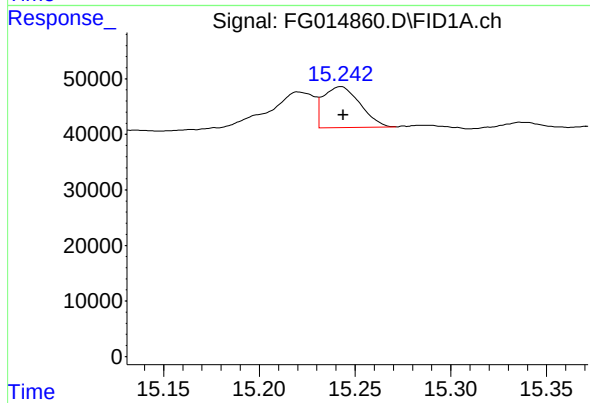

#14 n-Tetracosane (C24)


R.T.: 15.243 min
Delta R.T.: -0.001 min
Response: 97871
Conc: 0.78 ug/ml

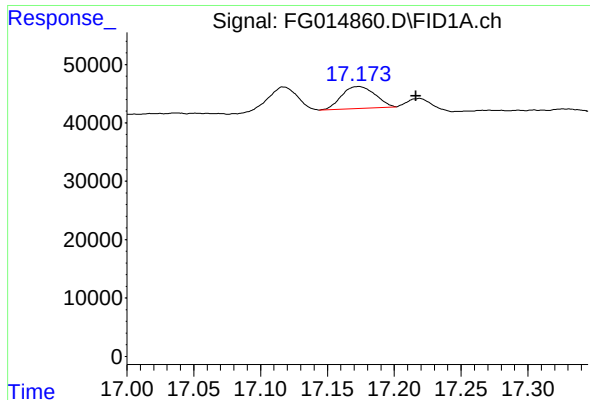

#16 n-Octacosane (C28)


R.T.: 17.173 min
Delta R.T.: -0.043 min
Response: 65040
Conc: 0.54 ug/ml

Instrument :
FID_G
ClientSampleId :

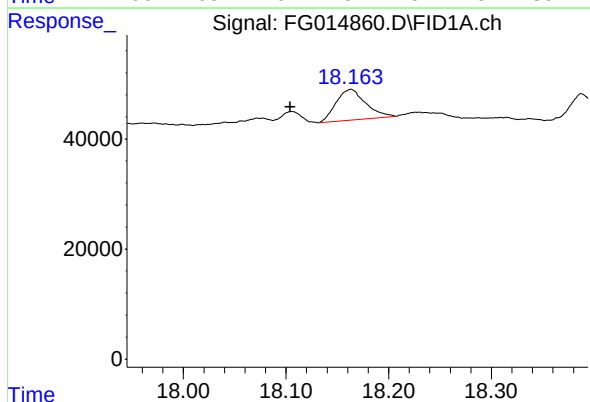


#17 n-Tricontane (C30)

R.T.: 18.163 min
Delta R.T.: 0.059 min
Response: 111005
Conc: 0.89 ug/ml

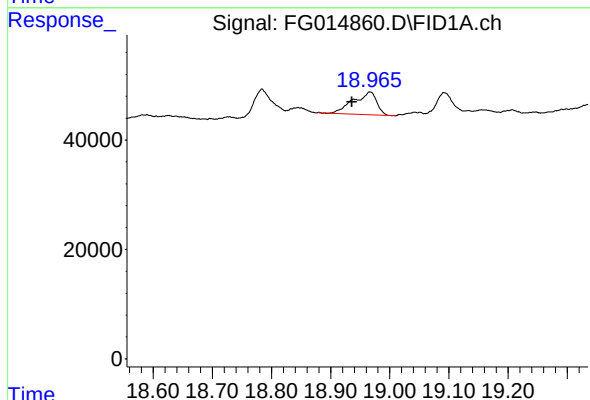

#18 n-Dotriacontane (C32)

R.T.: 18.967 min
Delta R.T.: 0.031 min
Response: 114677
Conc: 0.92 ug/ml

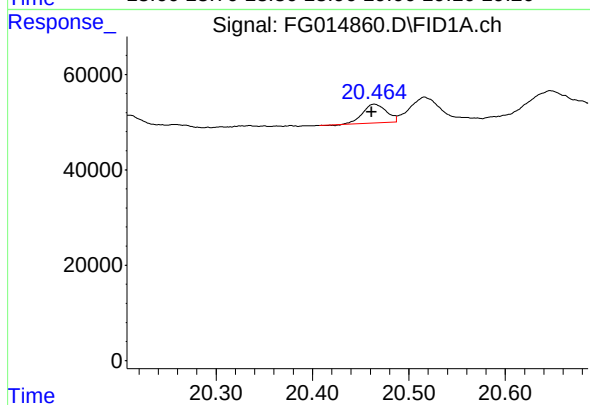

#20 n-Hexatriacontane (C36)

R.T.: 20.464 min
Delta R.T.: 0.003 min
Response: 66352
Conc: 0.72 ug/ml