

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111924AL\
Data File : FG014880.D
Signal(s) : FID1A.ch
Acq On : 19 Nov 2024 18:59
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 20 00:37:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 111424.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 16:33:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.103	55034	0.439 ug/ml
18) T	n-Dotriacontane (C32)	18.935	70202	0.564 ug/ml
19) T	n-Tetratriacontane (C34)	19.720	54186	0.502 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111924AL\
Data File : FG014880.D
Signal(s) : FID1A.ch
Acq On : 19 Nov 2024 18:59
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 20 00:37:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 111424.M
Quant Title : GC Extractables
QLast Update : Thu Nov 14 16:33:02 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

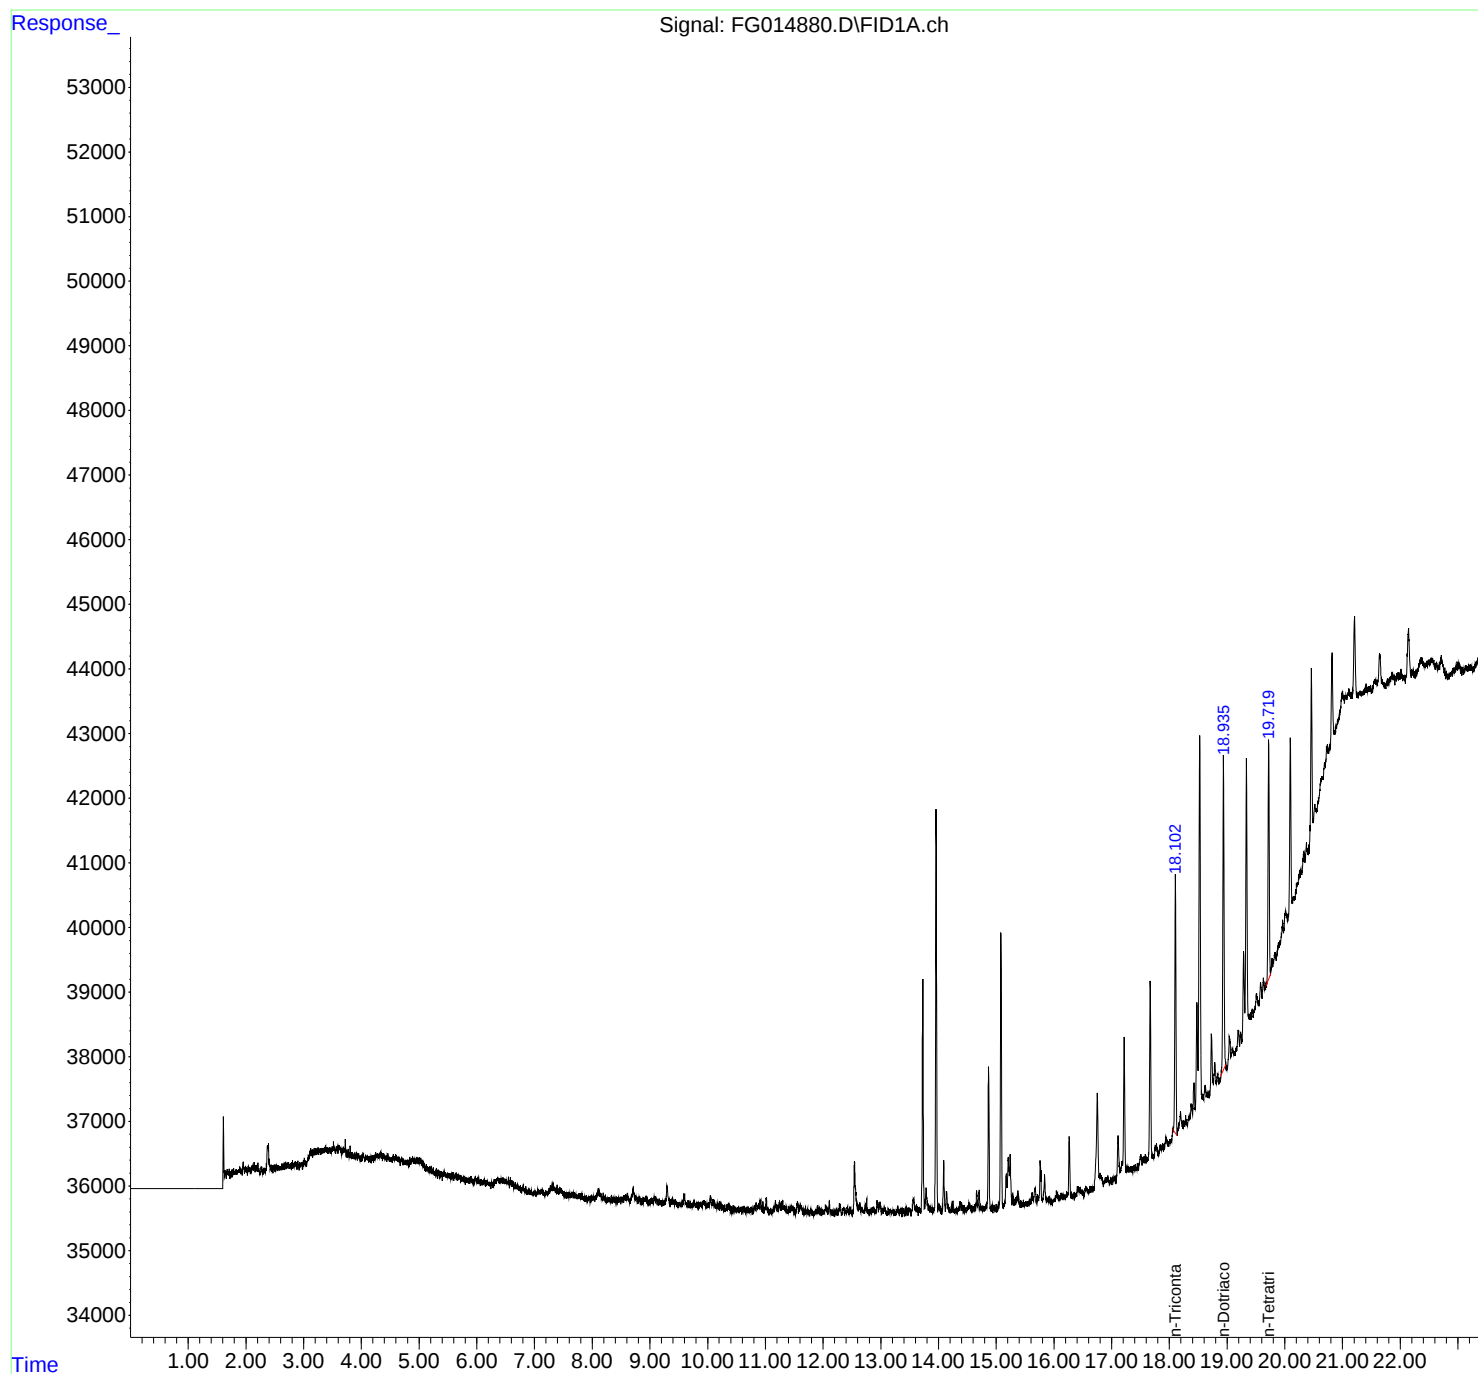


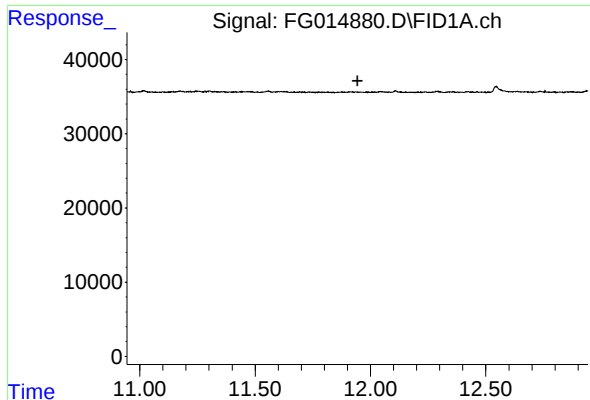

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.944 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

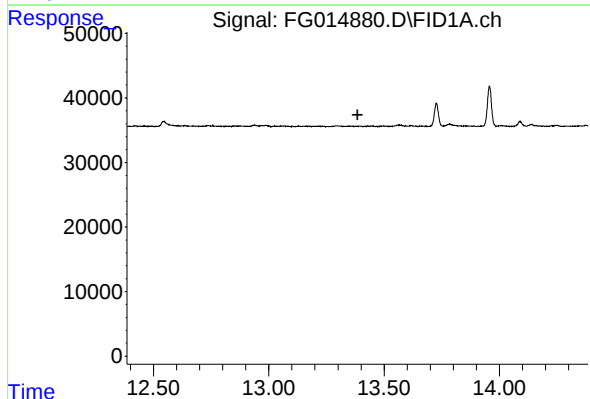


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.384 min
Response: 0
Conc: N.D.

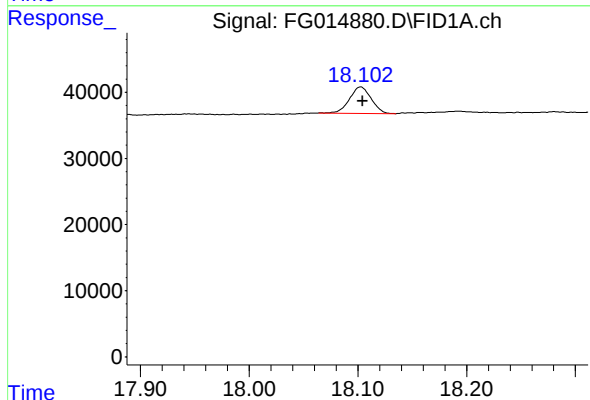


#17 n-Tricontane (C30)

R.T.: 18.103 min
Delta R.T.: -0.002 min
Response: 55034
Conc: 0.44 ug/ml

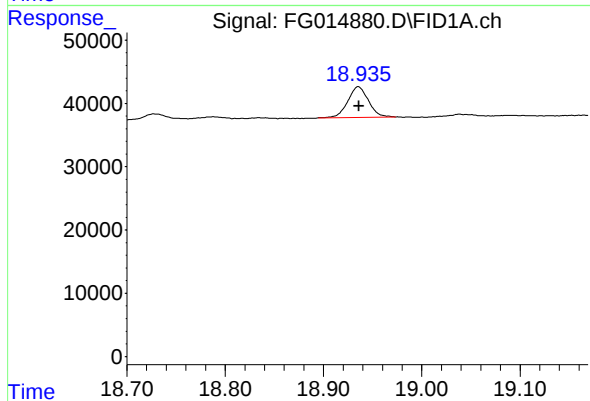

#18 n-Dotriacontane (C32)

R.T.: 18.935 min
Delta R.T.: 0.000 min
Response: 70202
Conc: 0.56 ug/ml

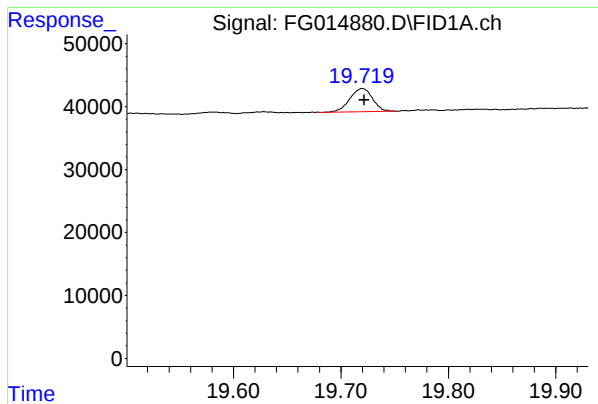

#19 n-Tetratriacontane (C34)

R.T.: 19.720 min

Delta R.T.: -0.002 min

Response: 54186

Conc: 0.50 ug/ml

Instrument :

FID_G

ClientSampleId :