

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112118\
 Data File : FG003026.D
 Signal(s) : FID1A.ch
 Acq On : 21 Nov 2018 13:13
 Operator : AJ\SJ
 Sample : J5763-03 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 21 16:51:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112018.M
 Quant Title :
 QLast Update : Wed Nov 21 01:39:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.709	833342	7.137 ug/ml
Target Compounds			
2) N-DECANE	4.420	39197	0.265 ug/ml
3) N-DODECANE	6.445	283274	1.918 ug/ml
4) N-TETRADECANE	8.244	497528	3.385 ug/ml
5) N-HEXADECANE	9.847	571316	3.937 ug/ml
6) N-OCTADECANE	11.293	565166	3.949 ug/ml
7) N-EICOSANE	12.605	590949	4.233 ug/ml
8) N-DOCOSANE	13.808	719396	5.284 ug/ml
10) N-TETRACOSANE	14.912	608482	4.598 ug/ml
11) N-HEXACOSANE	15.938	2624422	20.292 ug/ml
12) N-OCTACOSANE	16.892	1943061	15.316 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112118\
Data File : FG003026.D
Signal(s) : FID1A.ch
Acq On : 21 Nov 2018 13:13
Operator : AJ\SJ
Sample : J5763-03 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 21 16:51:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112018.M
Quant Title :
QLast Update : Wed Nov 21 01:39:34 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

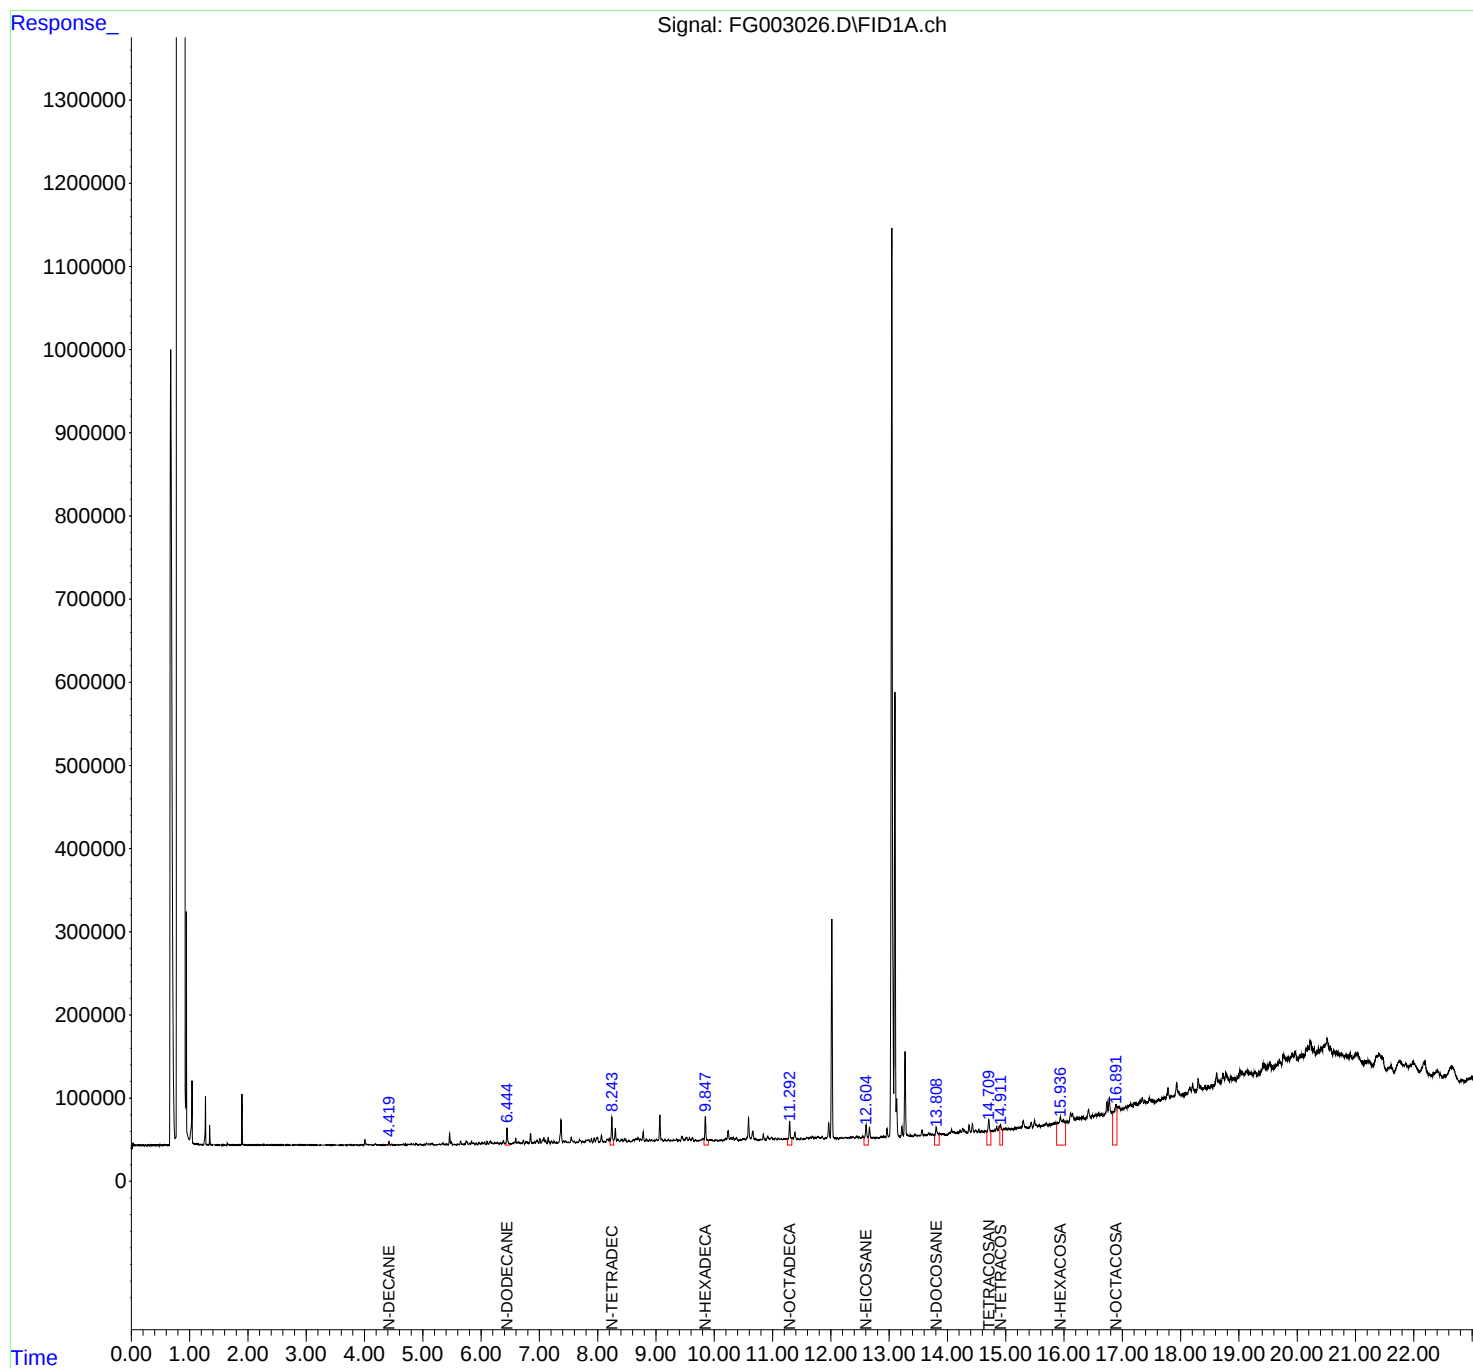

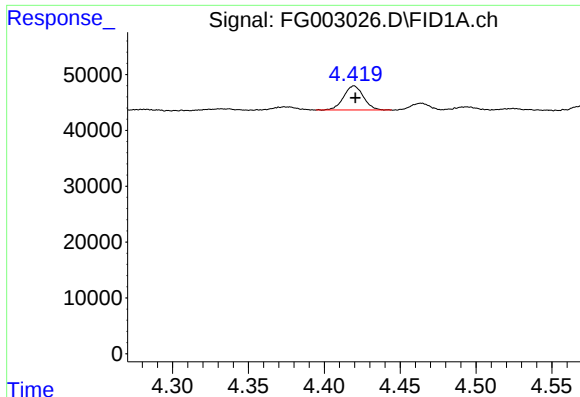


#2 N-DECANE

R.T.: 4.420 min
Delta R.T.: 0.000 min
Response: 39197
Conc: 0.27 ug/ml

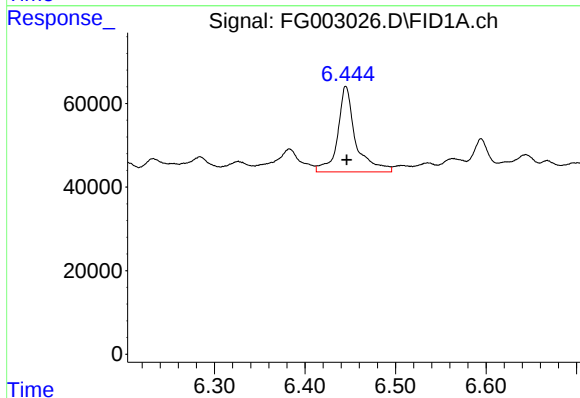


#3 N-DODECANE

R.T.: 6.445 min
Delta R.T.: 0.000 min
Response: 283274
Conc: 1.92 ug/ml

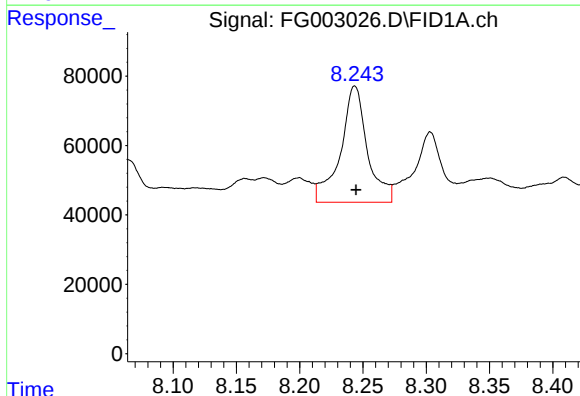


#4 N-TETRADECANE

R.T.: 8.244 min
Delta R.T.: 0.000 min
Response: 497528
Conc: 3.39 ug/ml

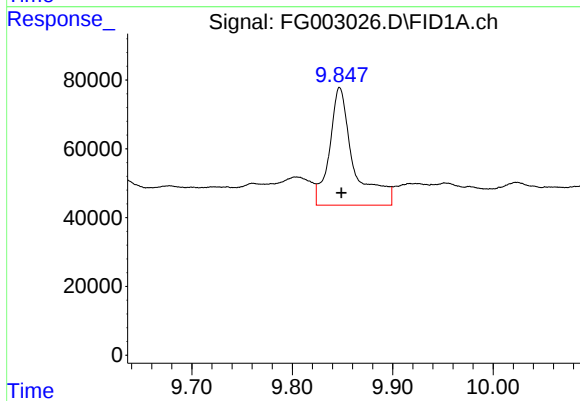


#5 N-HEXADECANE

R.T.: 9.847 min
Delta R.T.: -0.001 min
Response: 571316
Conc: 3.94 ug/ml

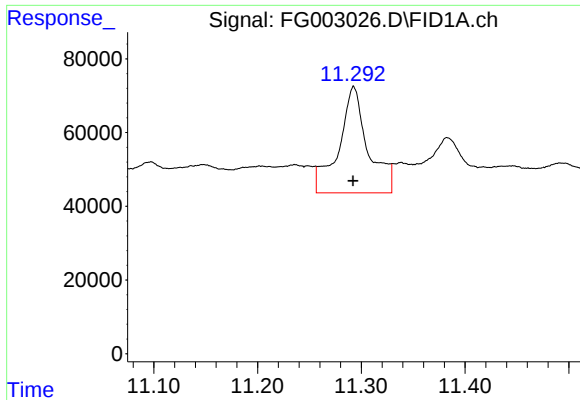


#6 N-OCTADECANE

R.T.: 11.293 min
Delta R.T.: 0.000 min
Response: 565166
Conc: 3.95 ug/ml

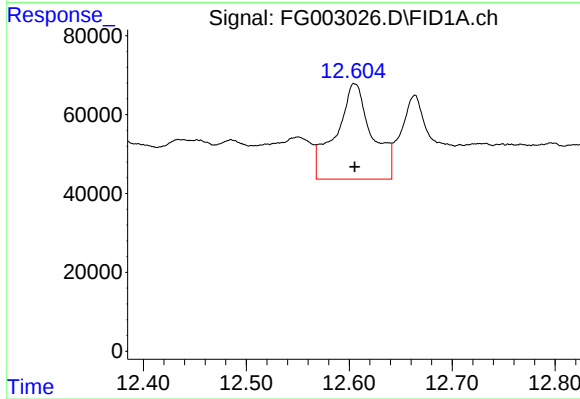


#7 N-EICOSANE

R.T.: 12.605 min
Delta R.T.: 0.000 min
Response: 590949
Conc: 4.23 ug/ml

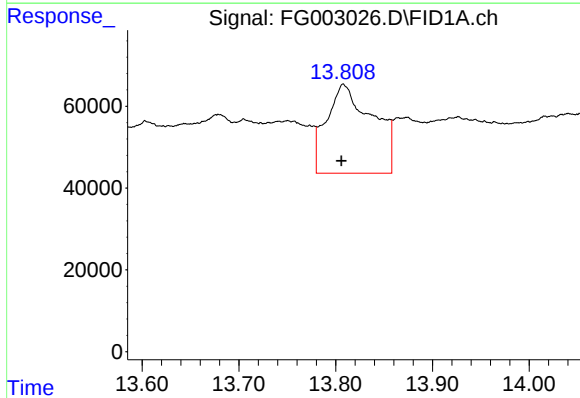


#8 N-DOCOSANE

R.T.: 13.808 min
Delta R.T.: 0.003 min
Response: 719396
Conc: 5.28 ug/ml

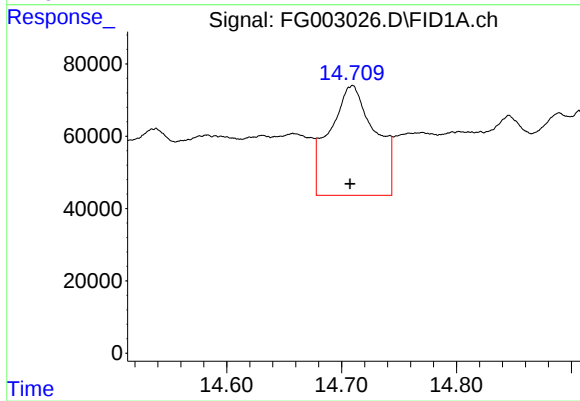


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.709 min
Delta R.T.: 0.002 min
Response: 833342
Conc: 7.14 ug/ml

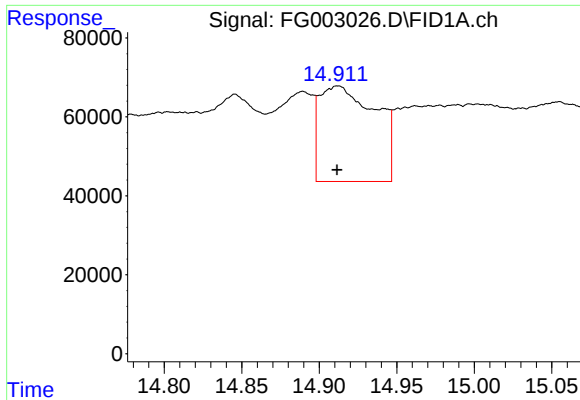


#10 N-TETRACOSANE

R.T.: 14.912 min
Delta R.T.: 0.000 min
Response: 608482
Conc: 4.60 ug/ml

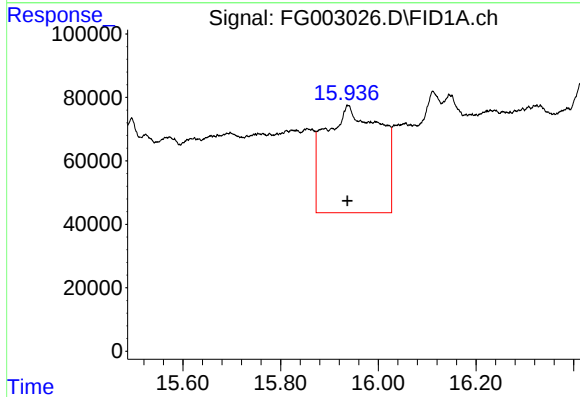

#11 N-HEXACOSANE

R.T.: 15.938 min
Delta R.T.: 0.002 min
Response: 2624422
Conc: 20.29 ug/ml

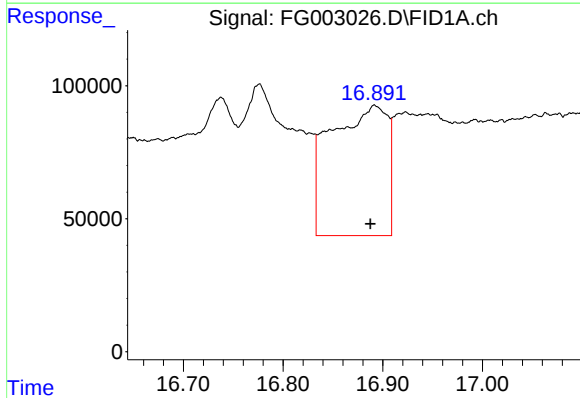

#12 N-OCTACOSANE

R.T.: 16.892 min
Delta R.T.: 0.005 min
Response: 1943061
Conc: 15.32 ug/ml