

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112118\
 Data File : FG003032.D
 Signal(s) : FID1A.ch
 Acq On : 21 Nov 2018 16:17
 Operator : AJ\SJ
 Sample : J5765-03 50X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 21 16:52:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112018.M
 Quant Title :
 QLast Update : Wed Nov 21 01:39:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.720	473076	4.052 ug/ml
Target Compounds			
2) N-DECANE	4.421	1979	0.013 ug/ml
4) N-TETRADECANE	8.229	27416	0.187 ug/ml
5) N-HEXADECANE	9.863	128063	0.882 ug/ml
6) N-OCTADECANE	11.295	24627	0.172 ug/ml
7) N-EICOSANE	12.615	122655	0.879 ug/ml
8) N-DOCOSANE	13.836	530085	3.894 ug/ml
10) N-TETRACOSANE	14.894	1460666	11.038 ug/ml
11) N-HEXACOSANE	15.950	547894	4.236 ug/ml
12) N-OCTACOSANE	16.898	928838	7.322 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112118\
Data File : FG003032.D
Signal(s) : FID1A.ch
Acq On : 21 Nov 2018 16:17
Operator : AJ\SJ
Sample : J5765-03 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 21 16:52:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112018.M
Quant Title :
QLast Update : Wed Nov 21 01:39:34 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

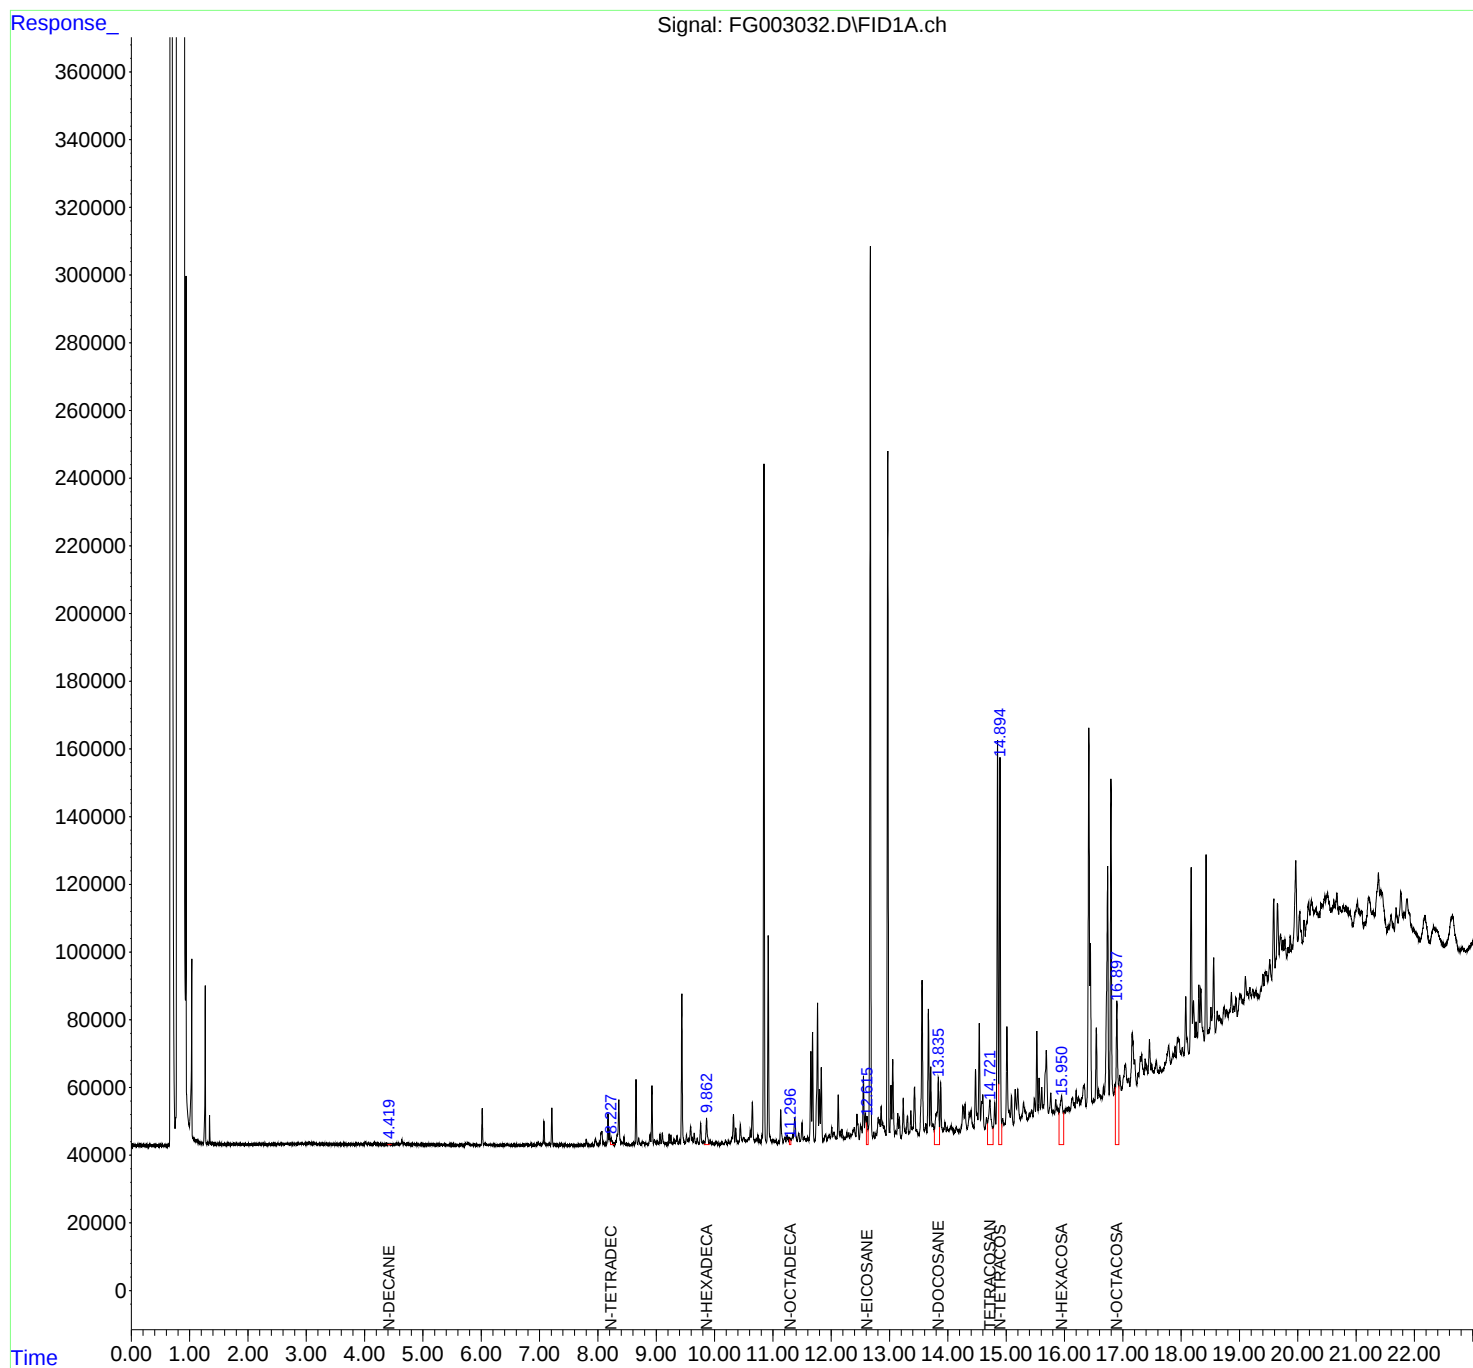

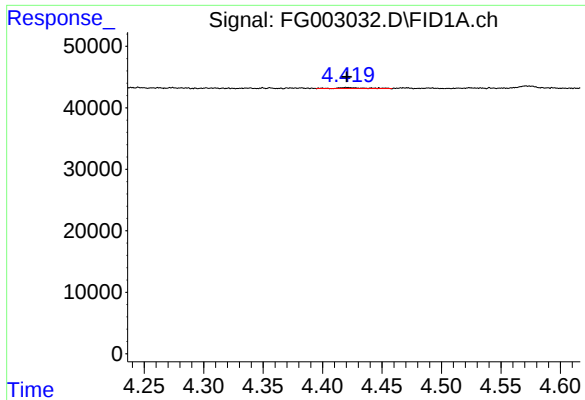


#2 N-DECANE

R.T.: 4.421 min
Delta R.T.: 0.000 min
Response: 1979
Conc: 0.01 ug/ml

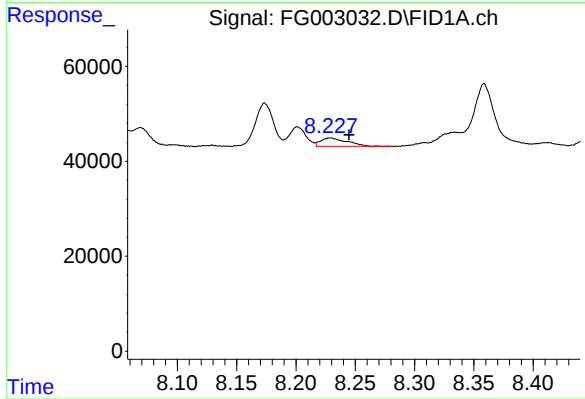


#4 N-TETRADECANE

R.T.: 8.229 min
Delta R.T.: -0.015 min
Response: 27416
Conc: 0.19 ug/ml

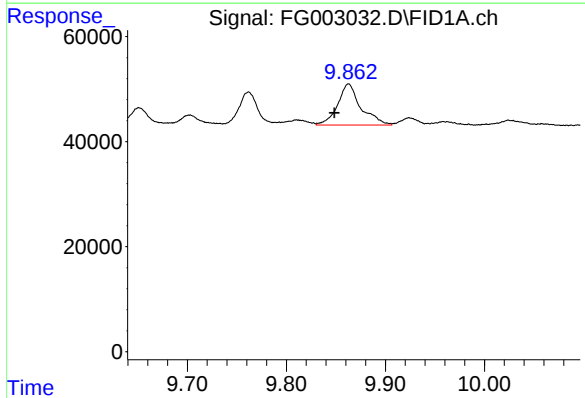


#5 N-HEXADECANE

R.T.: 9.863 min
Delta R.T.: 0.014 min
Response: 128063
Conc: 0.88 ug/ml

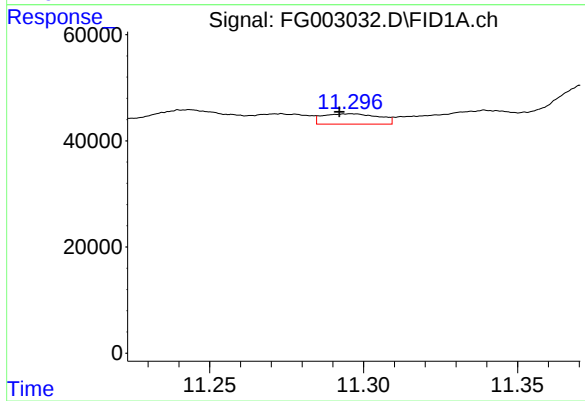


#6 N-OCTADECANE

R.T.: 11.295 min
Delta R.T.: 0.003 min
Response: 24627
Conc: 0.17 ug/ml

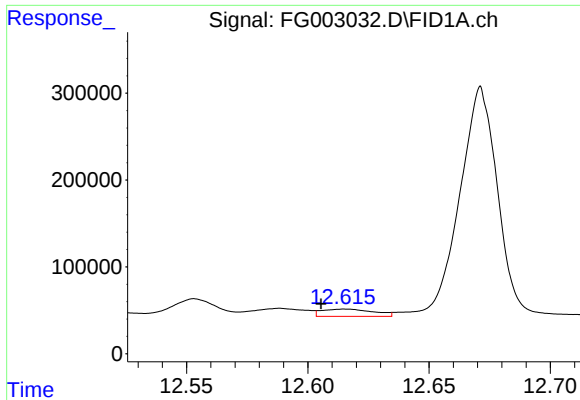


#7 N-EICOSANE

R.T.: 12.615 min
Delta R.T.: 0.010 min
Response: 122655
Conc: 0.88 ug/ml

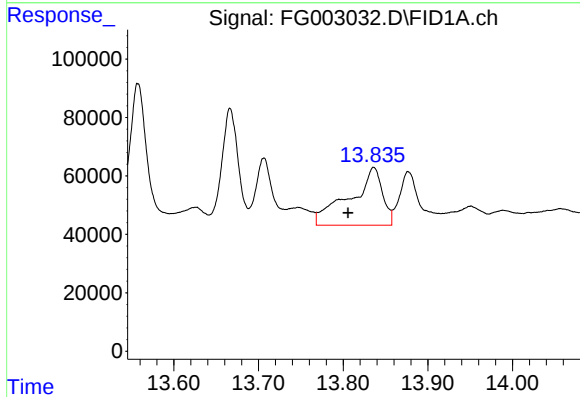


#8 N-DOCOSANE

R.T.: 13.836 min
Delta R.T.: 0.030 min
Response: 530085
Conc: 3.89 ug/ml

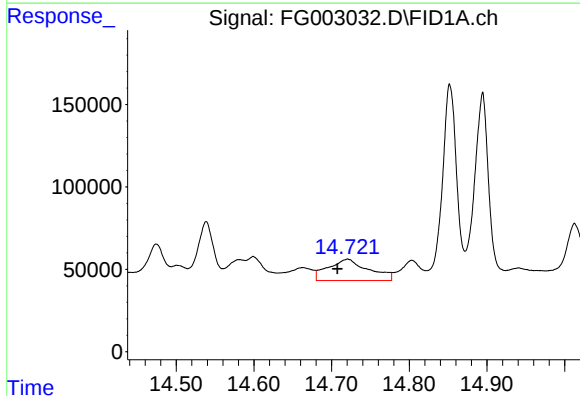


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.720 min
Delta R.T.: 0.013 min
Response: 473076
Conc: 4.05 ug/ml

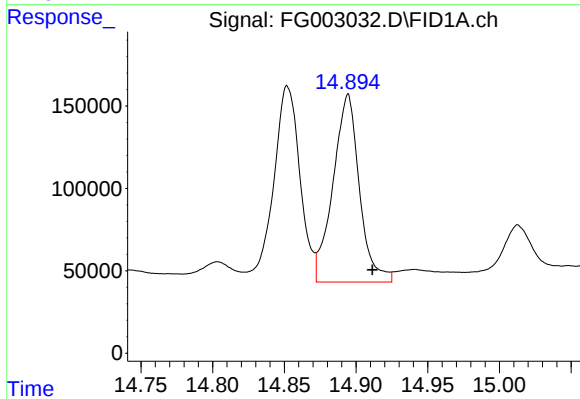


#10 N-TETRACOSANE

R.T.: 14.894 min
Delta R.T.: -0.017 min
Response: 1460666
Conc: 11.04 ug/ml

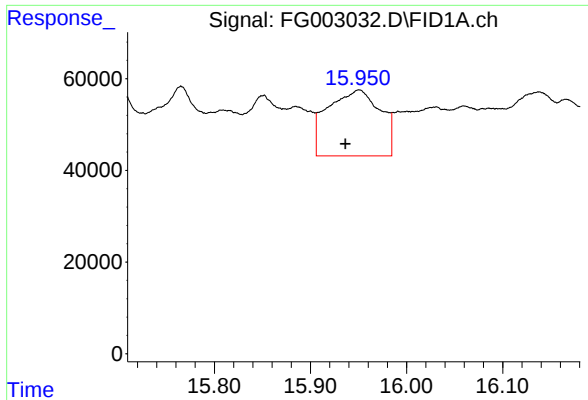

#11 N-HEXACOSANE

R.T.: 15.950 min
Delta R.T.: 0.014 min
Response: 547894
Conc: 4.24 ug/ml

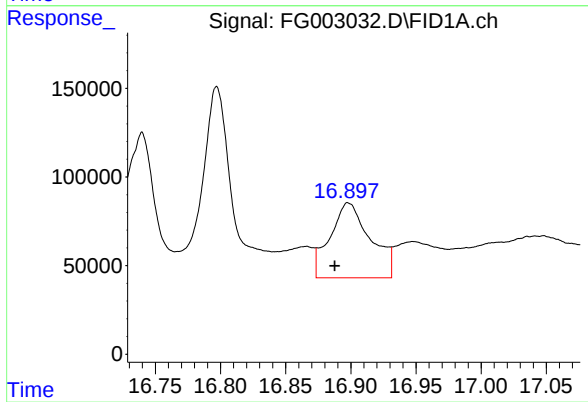

#12 N-OCTACOSANE

R.T.: 16.898 min
Delta R.T.: 0.011 min
Response: 928838
Conc: 7.32 ug/ml