

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112222\
Data File : FG011135.D
Signal(s) : FID1A.ch
Acq On : 22 Nov 2022 10:27
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 23 02:45:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
Quant Title :
QLast Update : Mon Nov 14 17:25:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.764	2338848	18.613 ug/ml
12)	N-OCTACOSANE	17.253	2320103	19.362 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112222\
Data File : FG011135.D
Signal(s) : FID1A.ch
Acq On : 22 Nov 2022 10:27
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 23 02:45:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
Quant Title :
QLast Update : Mon Nov 14 17:25:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

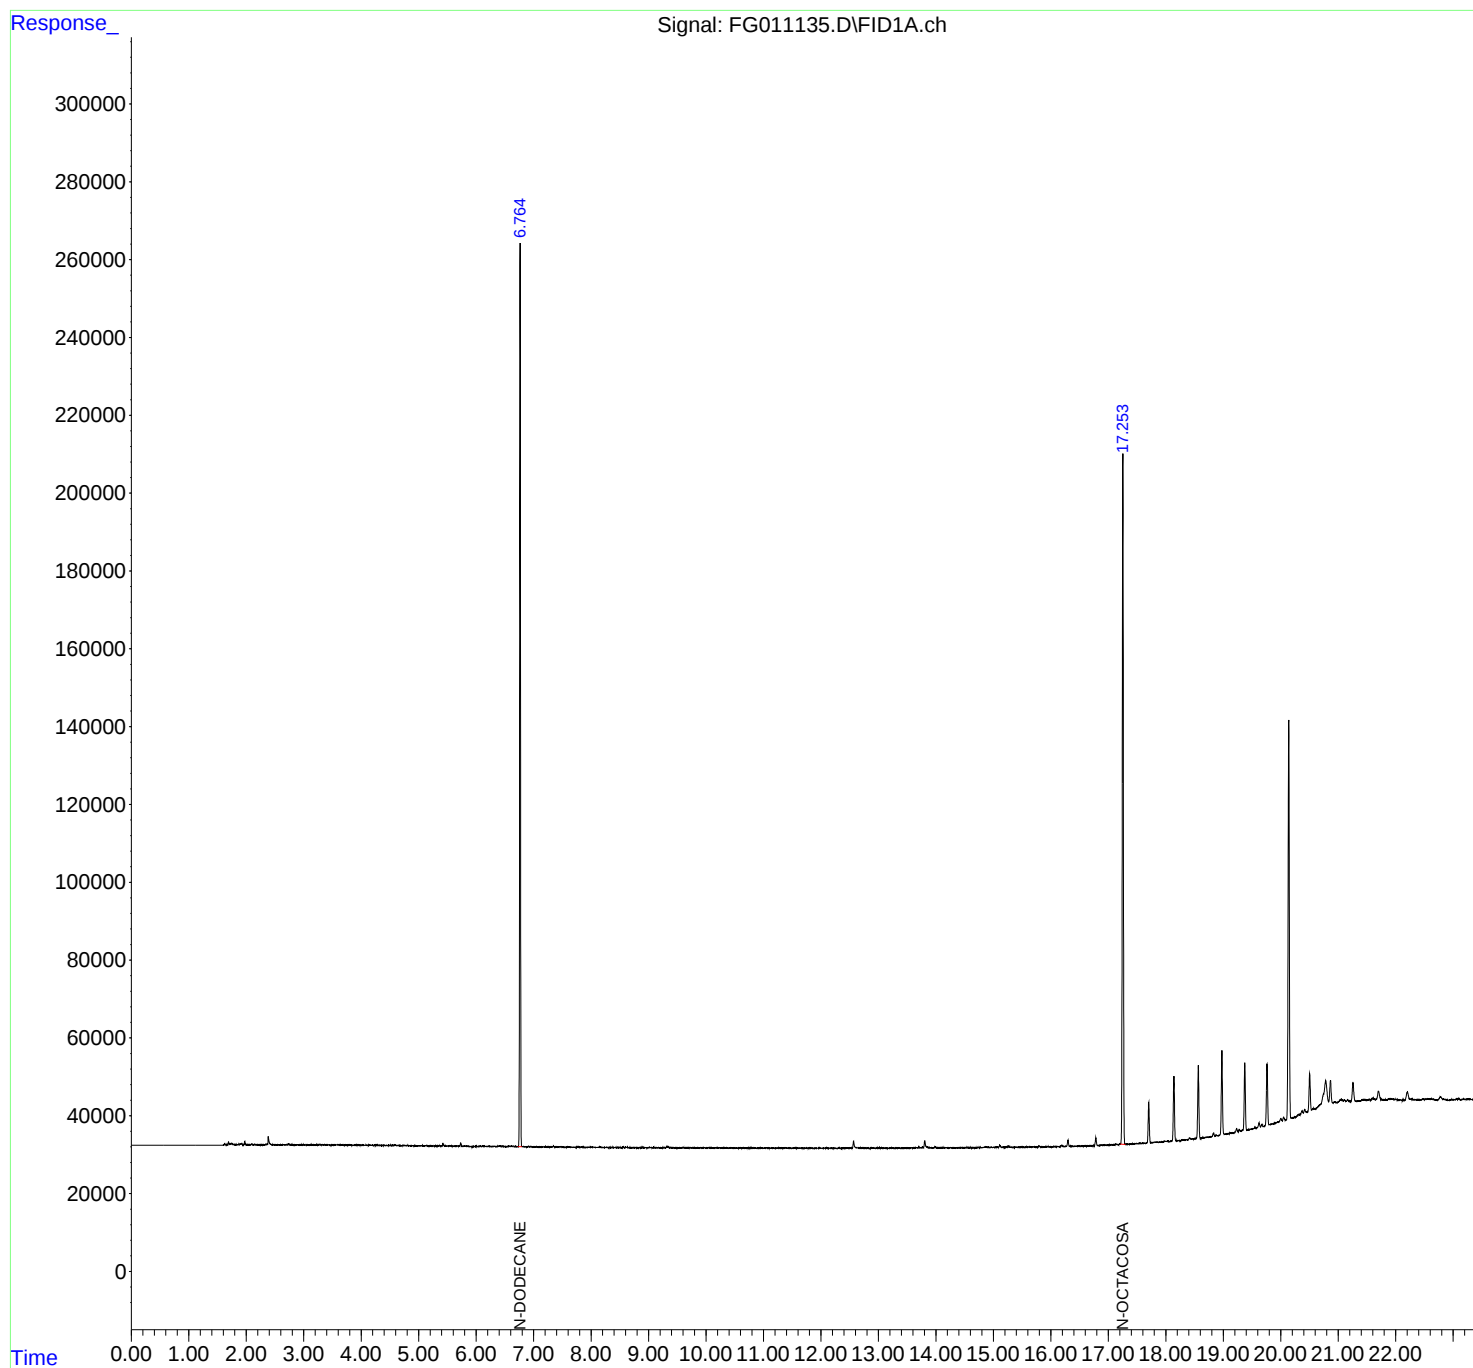


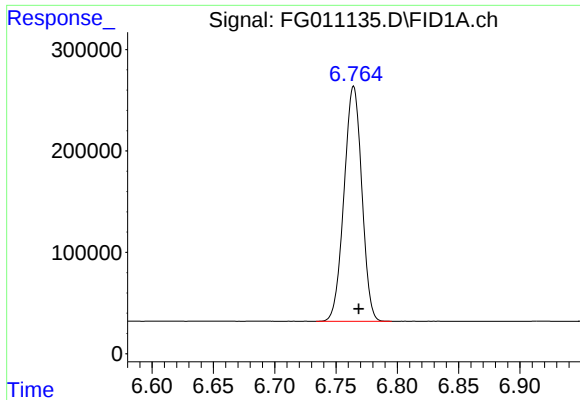

#3 N-DODECANE


R.T.: 6.764 min
Delta R.T.: -0.004 min
Response: 2338848
Conc: 18.61 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

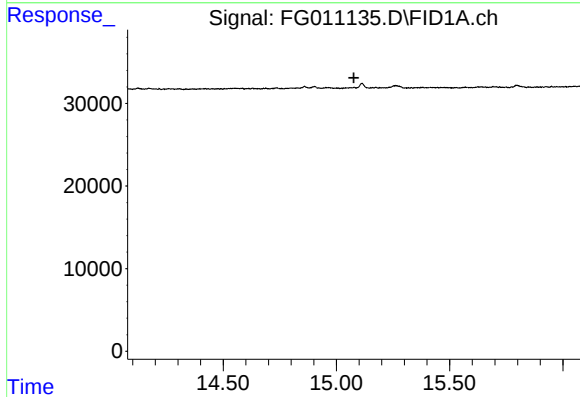

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.077 min
Response: 0
Conc: N.D.

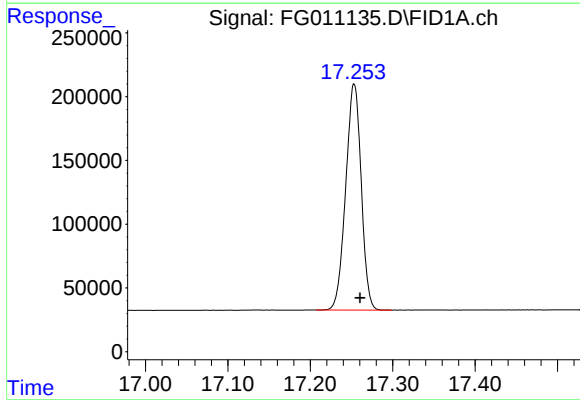

#12 N-OCTACOSANE

R.T.: 17.253 min
Delta R.T.: -0.007 min
Response: 2320103
Conc: 19.36 ug/ml