

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112321\
Data File : FG009091.D
Signal(s) : FID1A.ch
Acq On : 23 Nov 2021 15:36
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 24 01:02:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	17.839	64726	0.598 ug/ml
14)	N-DOTRIACONTANE	18.676	124726	1.213 ug/ml
15)	N-TETRATRIACONTANE	19.462	208957	2.113 ug/ml
17)	N-OCTATRIACONTANE	20.959	270545	2.917 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112321\
Data File : FG009091.D
Signal(s) : FID1A.ch
Acq On : 23 Nov 2021 15:36
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 24 01:02:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

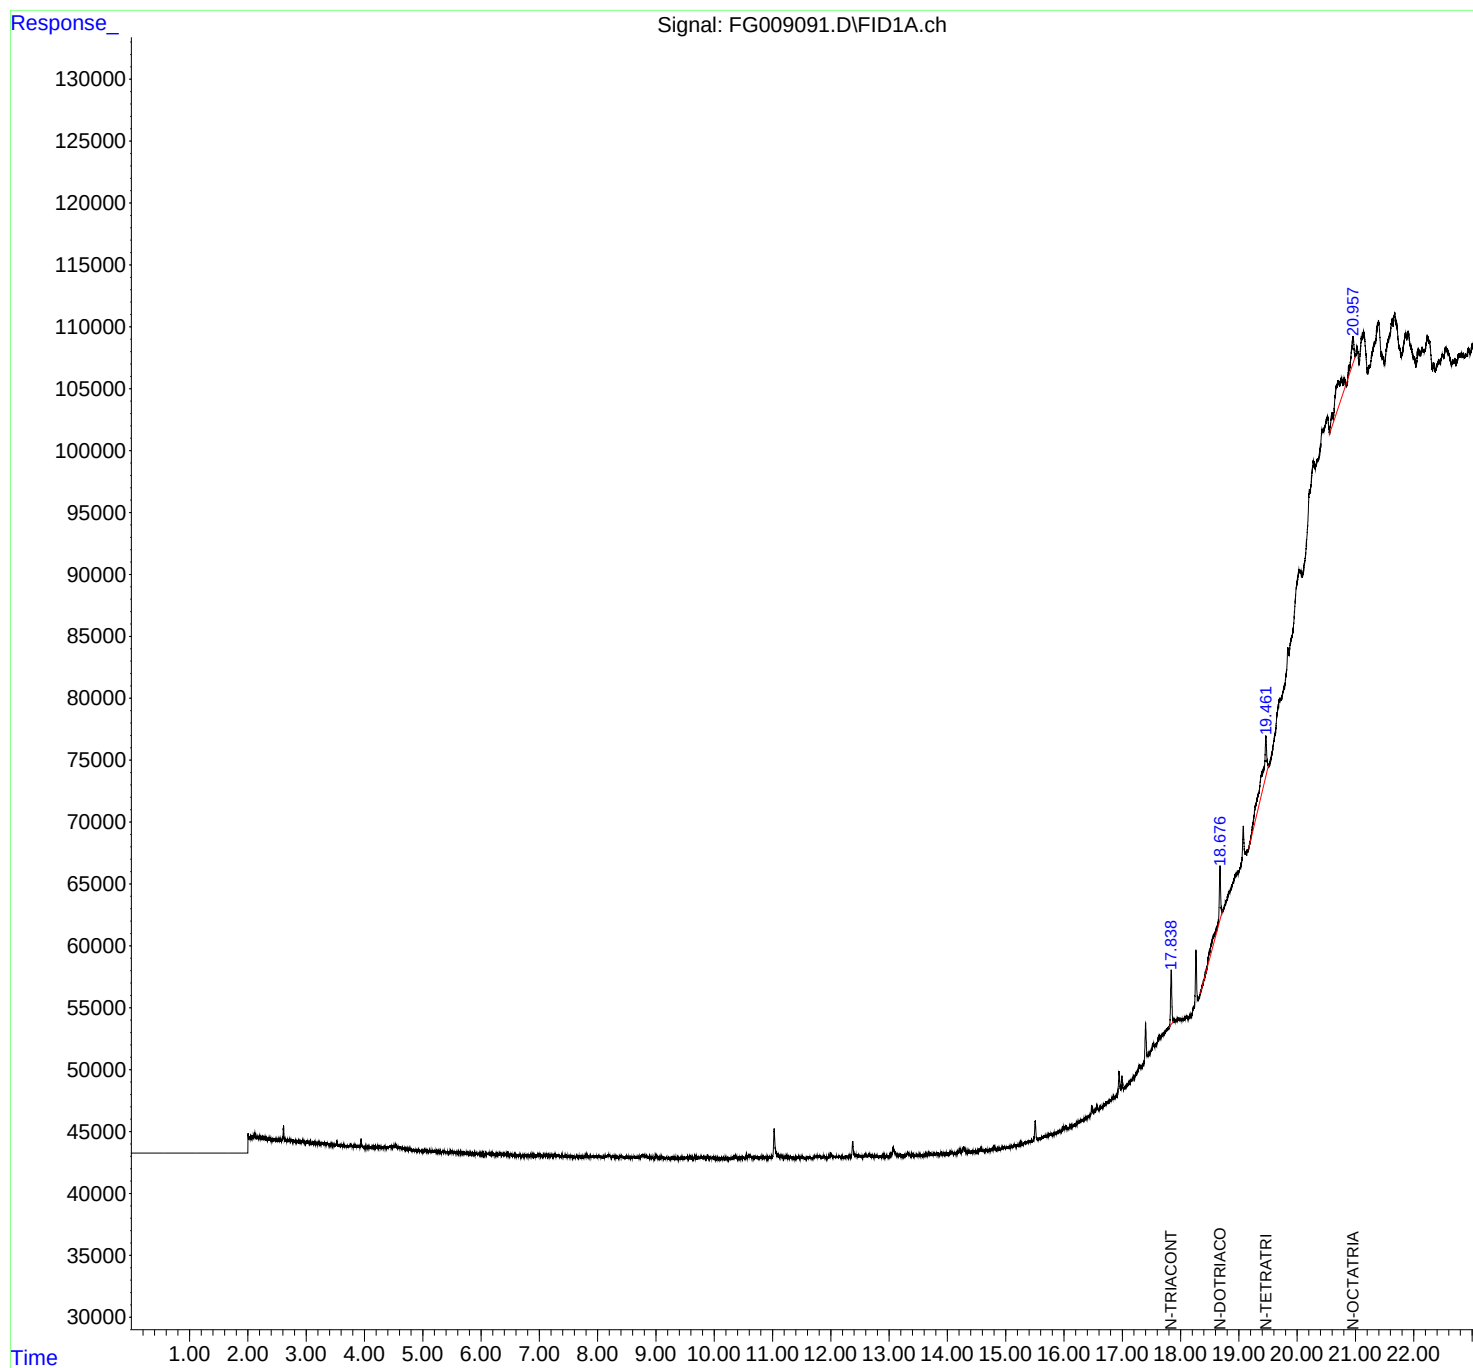


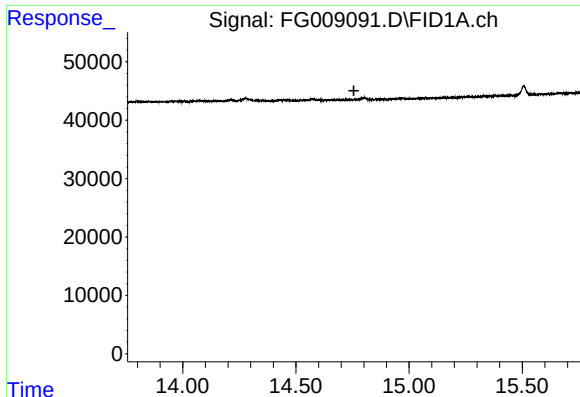

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.756 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

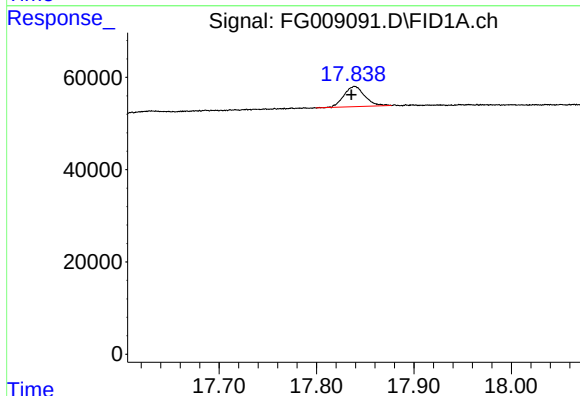


#13 N-TRIACONTANE

R.T.: 17.839 min
Delta R.T.: 0.003 min
Response: 64726
Conc: 0.60 ug/ml

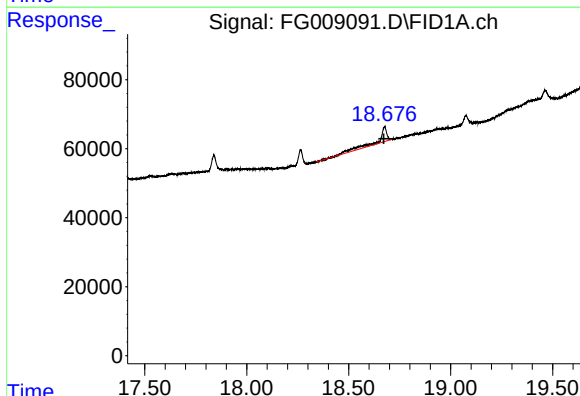


#14 N-DOTRIACONTANE

R.T.: 18.676 min
Delta R.T.: 0.005 min
Response: 124726
Conc: 1.21 ug/ml

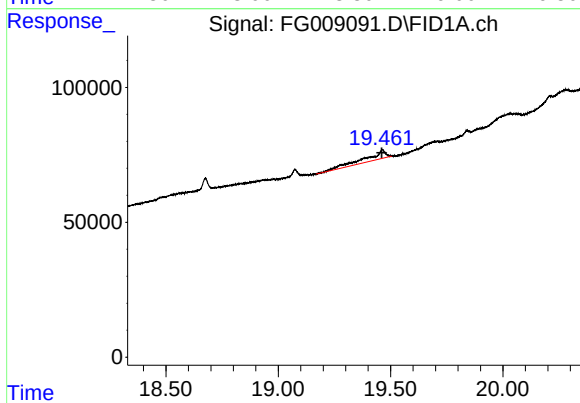

#15 N-TETRATRIACONTANE

R.T.: 19.462 min
Delta R.T.: 0.001 min
Response: 208957
Conc: 2.11 ug/ml

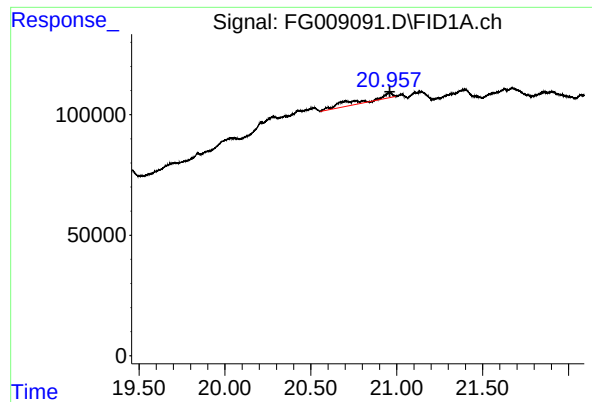

#17 N-OCTATRIACONTANE

R.T.: 20.959 min
Delta R.T.: -0.001 min
Response: 270545
Conc: 2.92 ug/ml

Instrument :

FID_G

ClientSampleId :