

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112321\
Data File : FG009099.D
Signal(s) : FID1A.ch
Acq On : 23 Nov 2021 19:39
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 24 01:02:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.672	53684	0.522 ug/ml
15)	N-TETRATRIACONTANE	19.459	58802	0.595 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112321\
Data File : FG009099.D
Signal(s) : FID1A.ch
Acq On : 23 Nov 2021 19:39
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 24 01:02:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

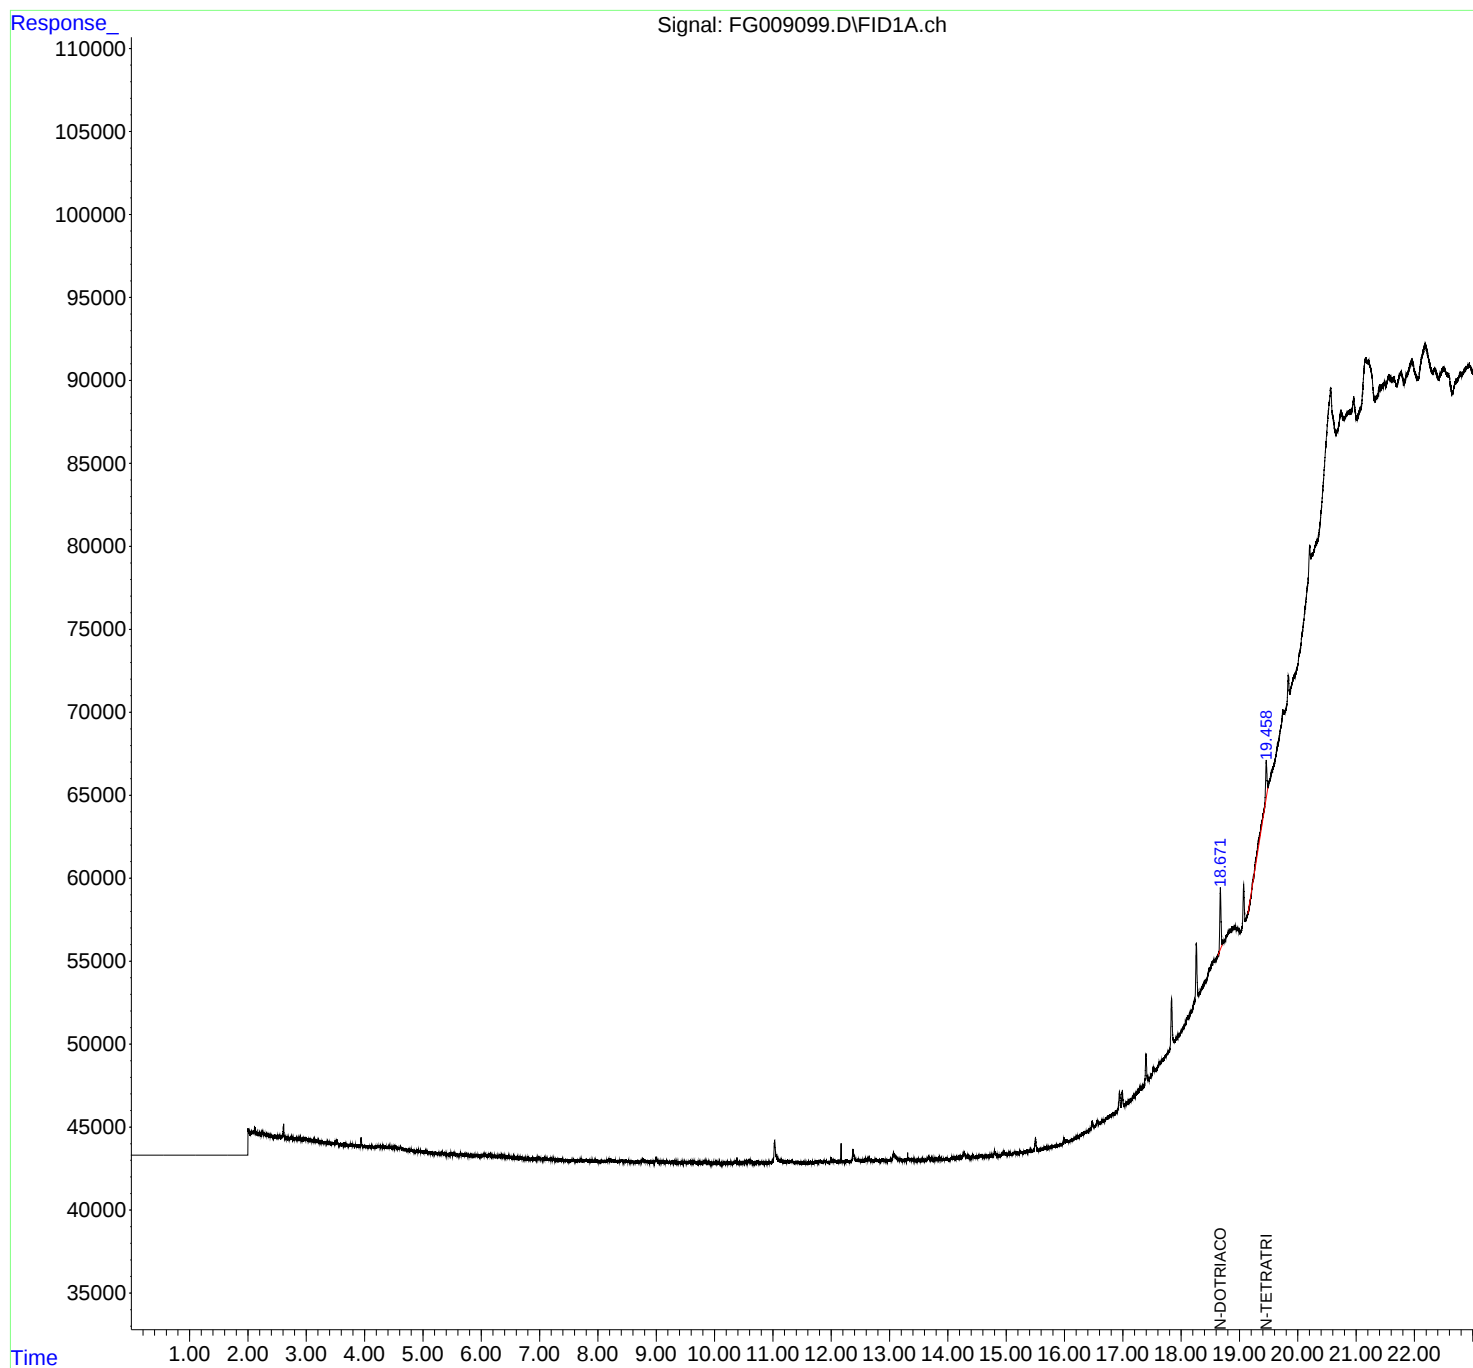


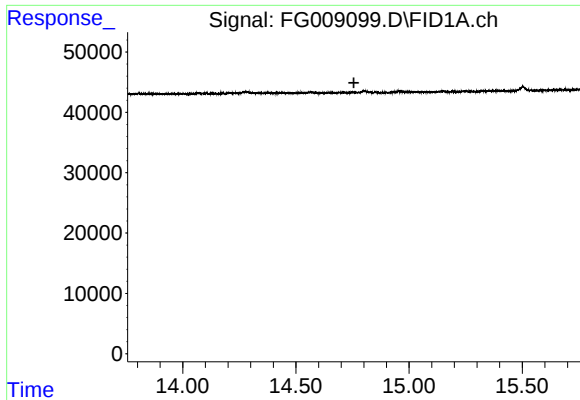

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.756 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

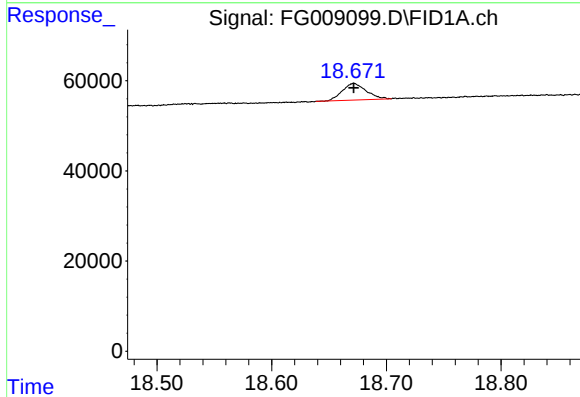

#14 N-DOTRIACONTANE

R.T.: 18.672 min
Delta R.T.: 0.000 min
Response: 53684
Conc: 0.52 ug/ml

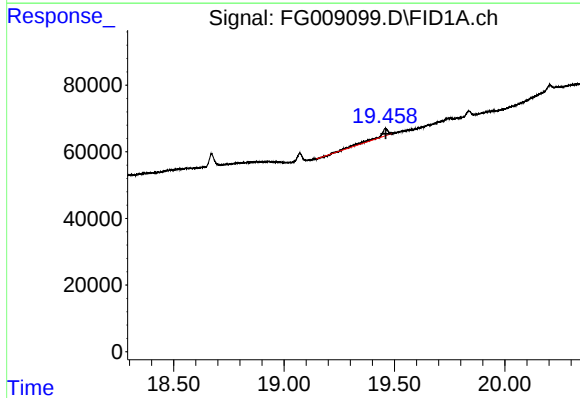

#15 N-TETRATRIACONTANE

R.T.: 19.459 min
Delta R.T.: -0.002 min
Response: 58802
Conc: 0.59 ug/ml