

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112520\
 Data File : FG007384.D
 Signal(s) : FID1A.ch
 Acq On : 25 Nov 2020 11:22
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 26 00:42:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
 Quant Title :
 QLast Update : Tue Nov 03 02:04:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.463	4833188	34.507 ug/ml
6) N-OCTADECANE	11.316	86963	0.601 ug/ml
12) N-OCTACOSANE	16.914	4314228	32.488 ug/ml
13) N-TRIACONTANE	17.800	331240	2.576 ug/ml
14) N-DOTRIACONTANE	18.634	462672	3.902 ug/ml
15) N-TETRATRIACONTANE	19.420	343818	3.558 ug/ml
16) N-HEXATRIACONTANE	20.162	251357	3.268 ug/ml
17) N-OCTATRIACONTANE	20.913	134811	2.044 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112520\
Data File : FG007384.D
Signal(s) : FID1A.ch
Acq On : 25 Nov 2020 11:22
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 26 00:42:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

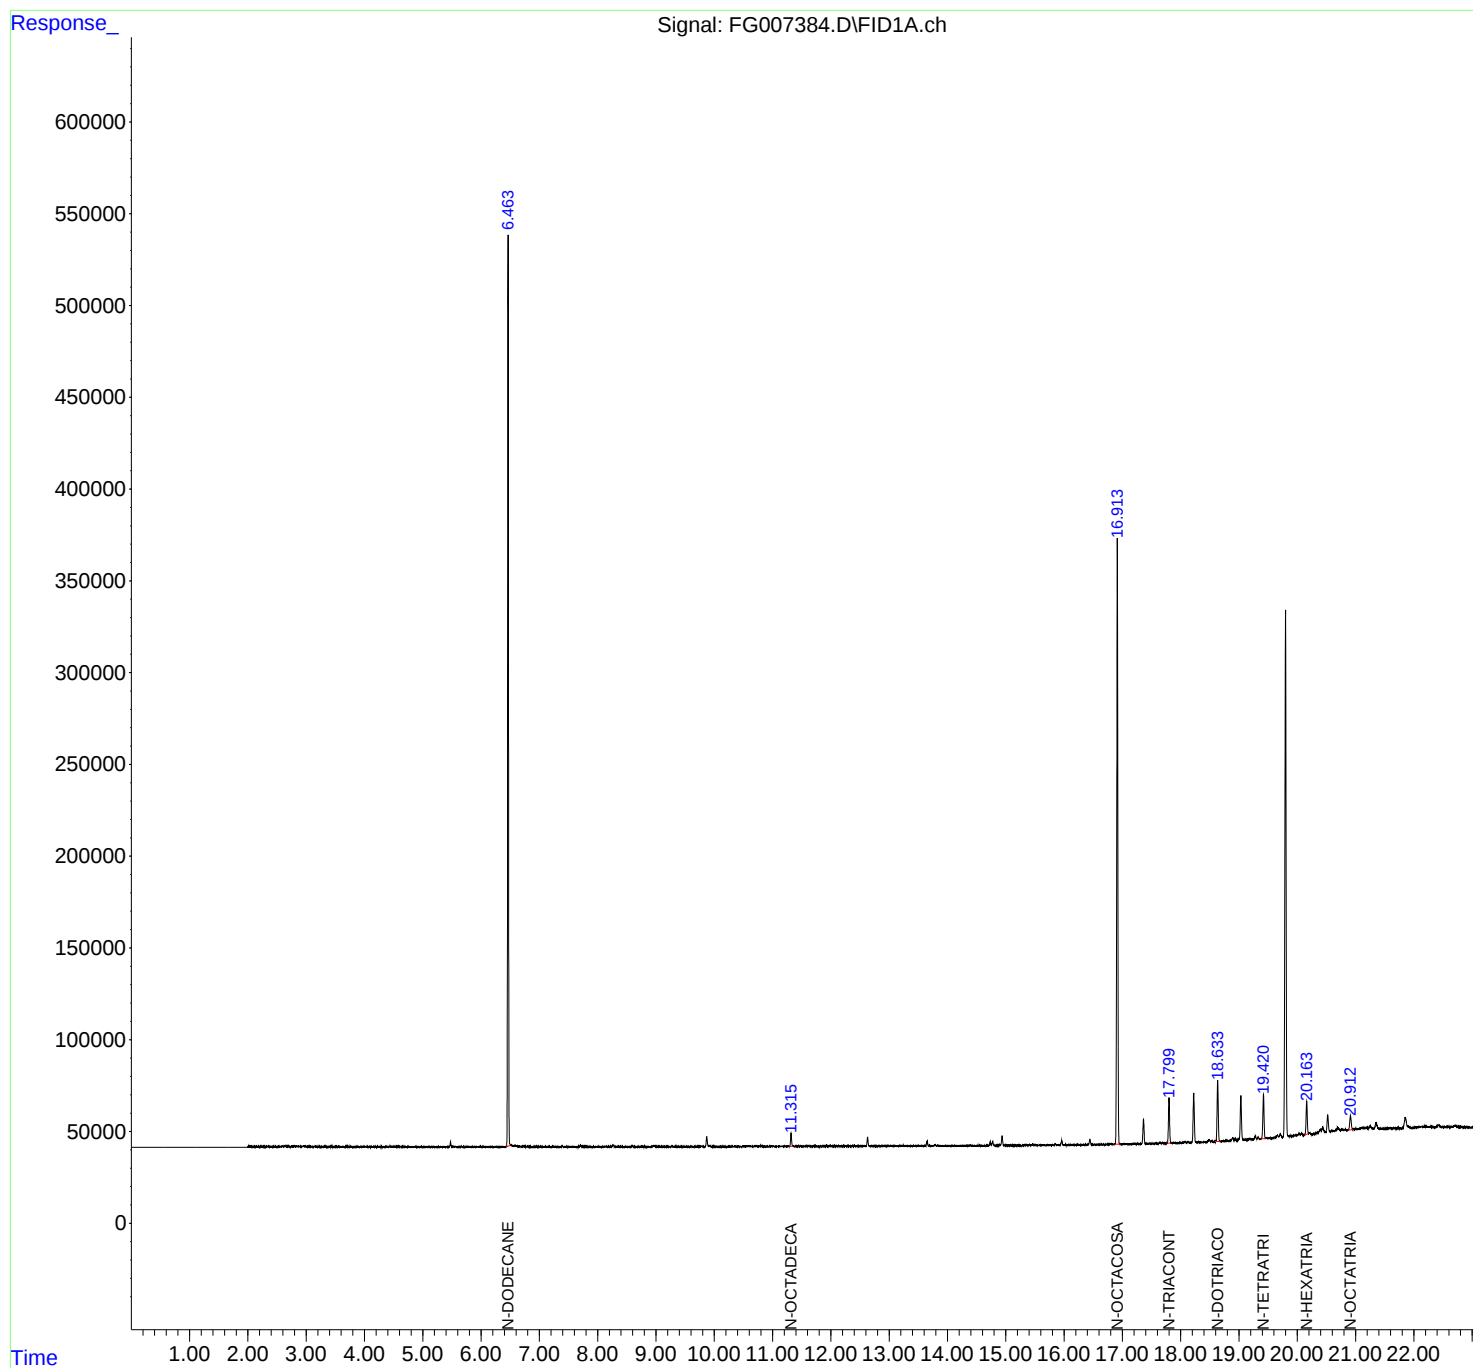


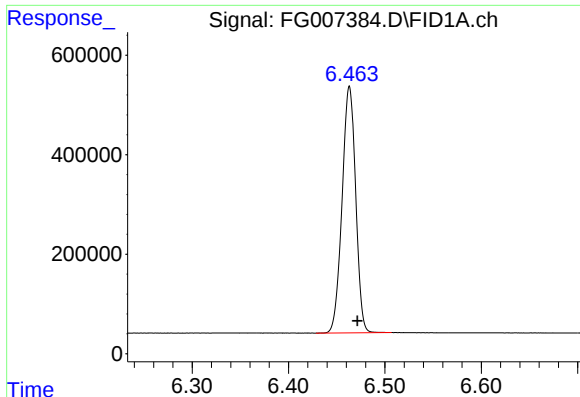

#3 N-DODECANE


R.T.: 6.463 min
Delta R.T.: -0.008 min
Response: 4833188
Conc: 34.51 ug/ml

Instrument :
FID_G
ClientSampleId :

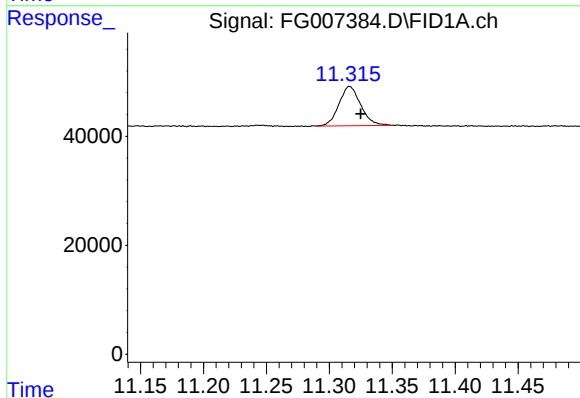


#6 N-OCTADECANE

R.T.: 11.316 min
Delta R.T.: -0.009 min
Response: 86963
Conc: 0.60 ug/ml

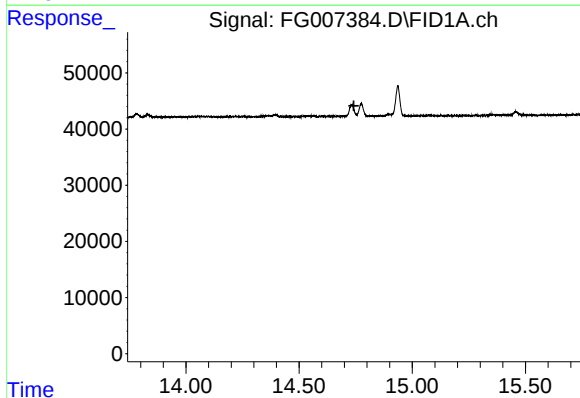


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.742 min
Response: 0
Conc: N.D.

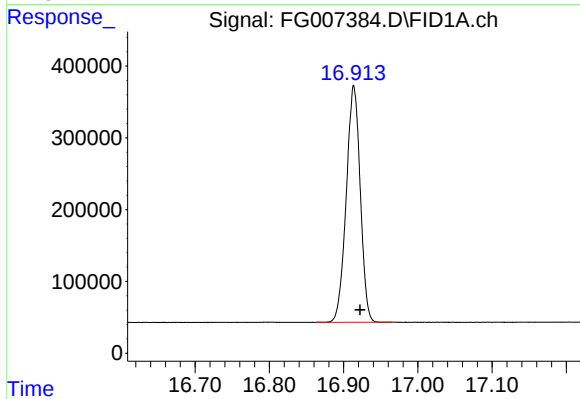

#12 N-OCTACOSANE


R.T.: 16.914 min
Delta R.T.: -0.008 min
Response: 4314228
Conc: 32.49 ug/ml

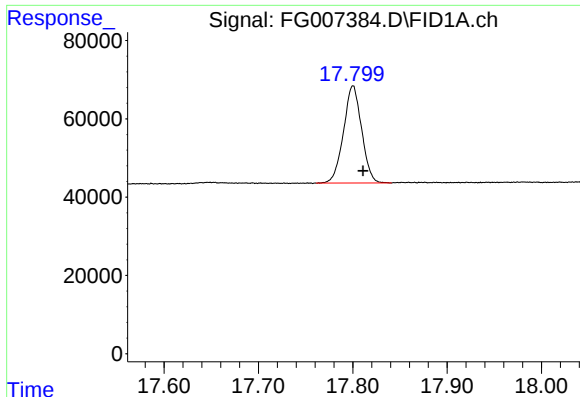

#13 N-TRIACONTANE


R.T.: 17.800 min
Delta R.T.: -0.011 min
Response: 331240
Conc: 2.58 ug/ml

Instrument :
FID_G
ClientSampleId :

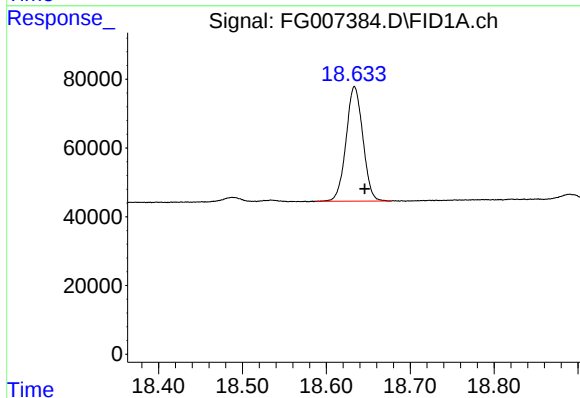


#14 N-DOTRIACONTANE

R.T.: 18.634 min
Delta R.T.: -0.012 min
Response: 462672
Conc: 3.90 ug/ml

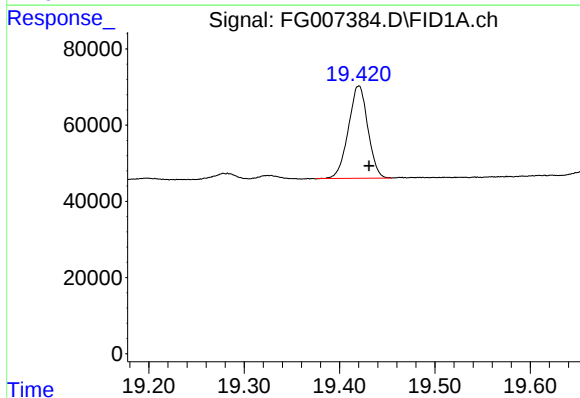


#15 N-TETRATRIACONTANE

R.T.: 19.420 min
Delta R.T.: -0.011 min
Response: 343818
Conc: 3.56 ug/ml

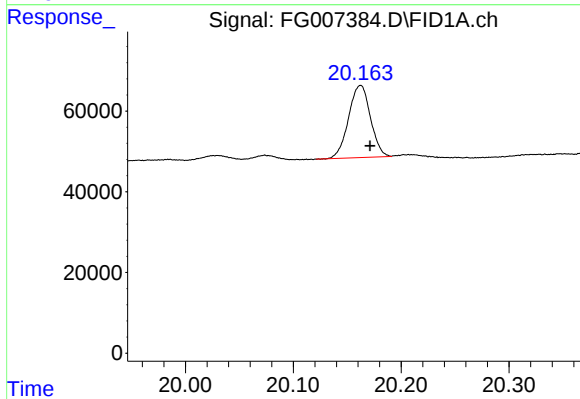

#16 N-HEXATRIACONTANE

R.T.: 20.162 min
Delta R.T.: -0.009 min
Response: 251357
Conc: 3.27 ug/ml

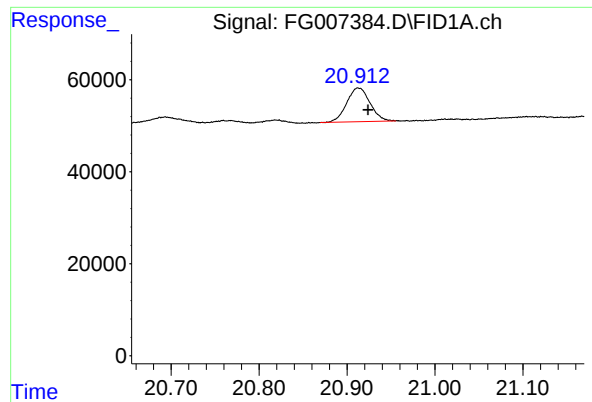

#17 N-OCTATRIACONTANE

R.T.: 20.913 min
Delta R.T.: -0.011 min
Response: 134811
Conc: 2.04 ug/ml

Instrument :
FID_G
ClientSampleId :