

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112520\
 Data File : FG007389.D
 Signal(s) : FID1A.ch
 Acq On : 25 Nov 2020 14:26
 Operator : DD\AJ
 Sample : L4891-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 26 00:43:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
 Quant Title :
 QLast Update : Tue Nov 03 02:04:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.743	1666108	13.543 ug/ml
Target Compounds			
4) N-TETRADECANE	8.334f	816828	5.793 ug/ml
7) N-EICOSANE	12.707f	396216	2.763 ug/ml
10) N-TETRACOSANE	14.932	251170	1.799 ug/ml
11) N-HEXACOSANE	15.970	121388	0.892 ug/ml
12) N-OCTACOSANE	16.934	142241	1.071 ug/ml
13) N-TRIACONTANE	17.815	507631	3.947 ug/ml
14) N-DOTRIACONTANE	18.642	669228	5.644 ug/ml
15) N-TETRATRIACONTANE	19.433	1556540	16.107 ug/ml
16) N-HEXATRIACONTANE	20.176	2465599	32.059 ug/ml
17) N-OCTATRIACONTANE	20.953	1666402	25.268 ug/ml
18) N-TETRACONTANE	21.859	180072	2.804 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112520\
Data File : FG007389.D
Signal(s) : FID1A.ch
Acq On : 25 Nov 2020 14:26
Operator : DD\AJ
Sample : L4891-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 26 00:43:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

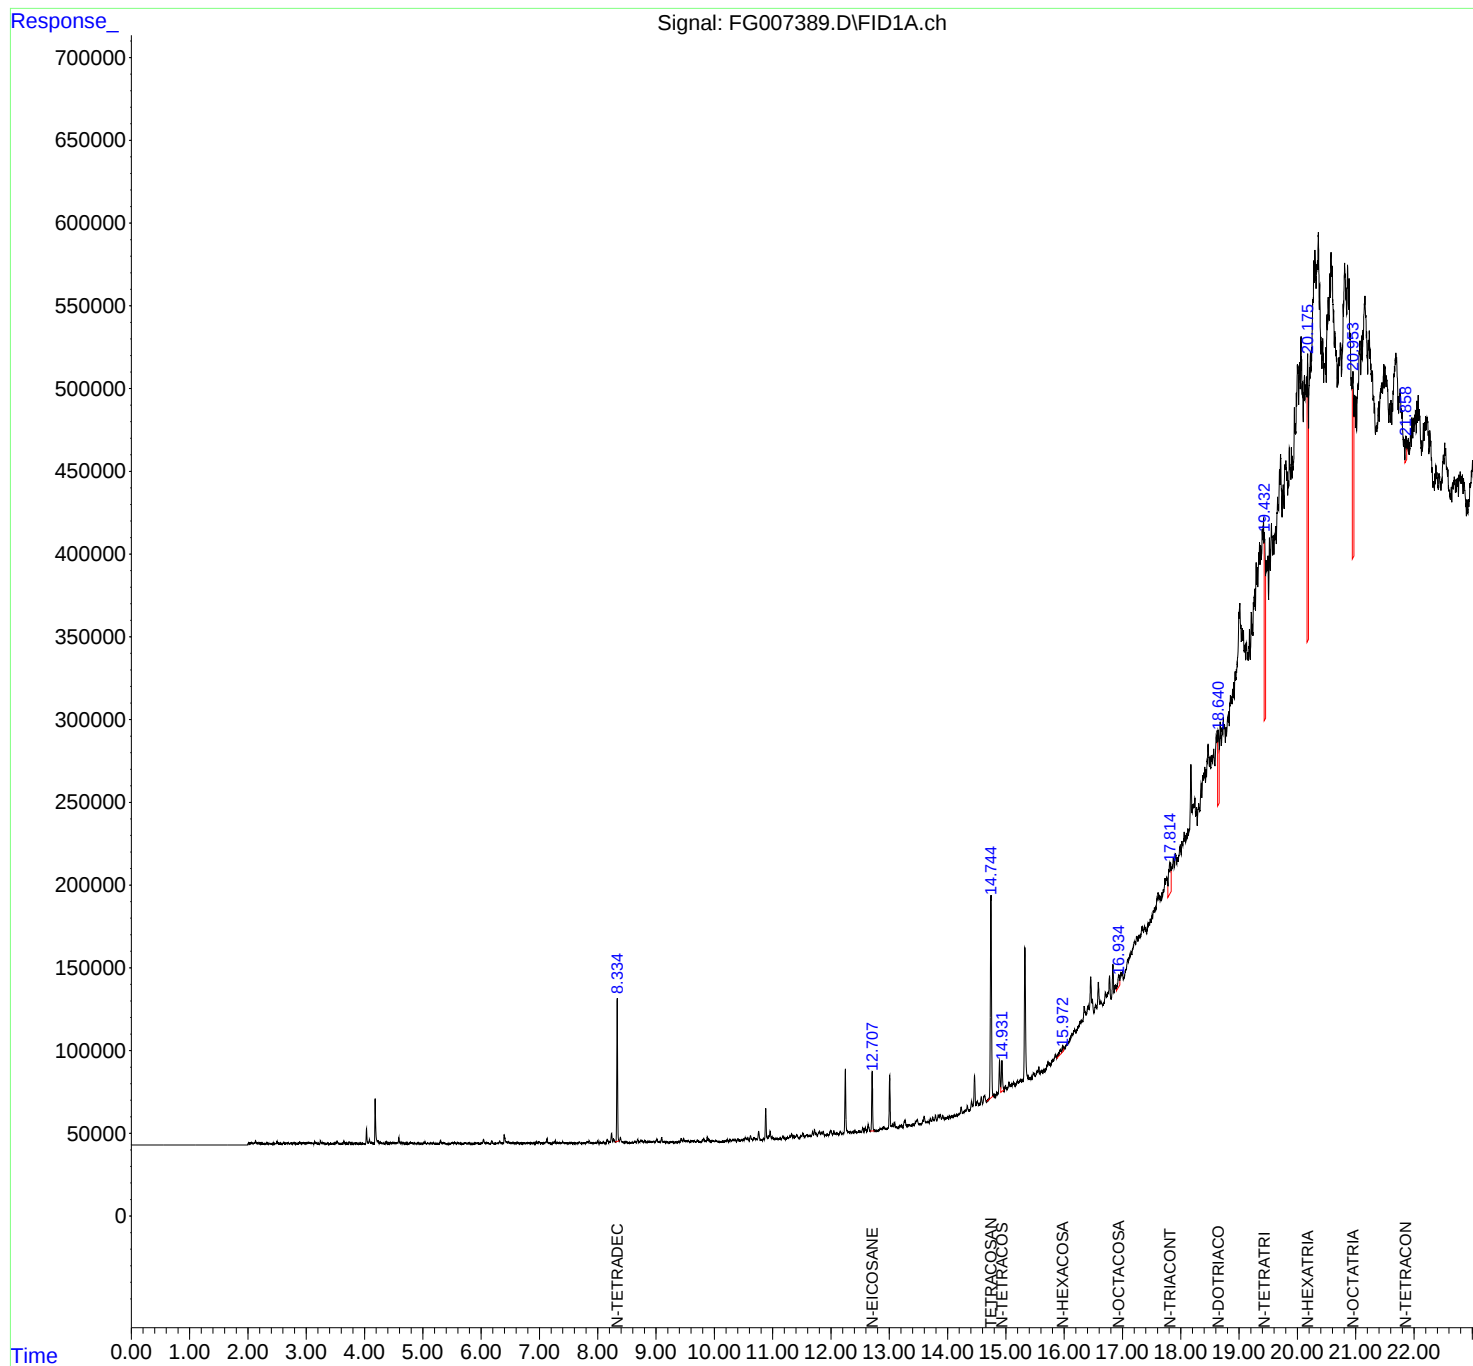


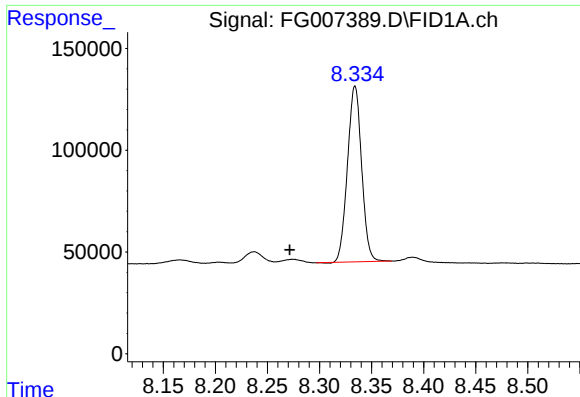

#4 N-TETRADECANE


R.T.: 8.334 min
Delta R.T.: 0.063 min
Response: 816828
Conc: 5.79 ug/ml

Instrument :
FID_G
ClientSampleId :

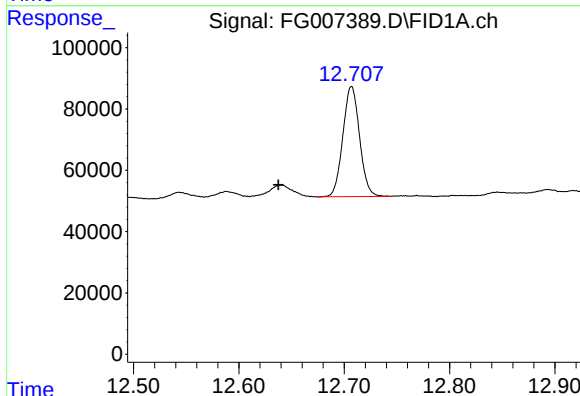


#7 N-EICOSANE

R.T.: 12.707 min
Delta R.T.: 0.069 min
Response: 396216
Conc: 2.76 ug/ml

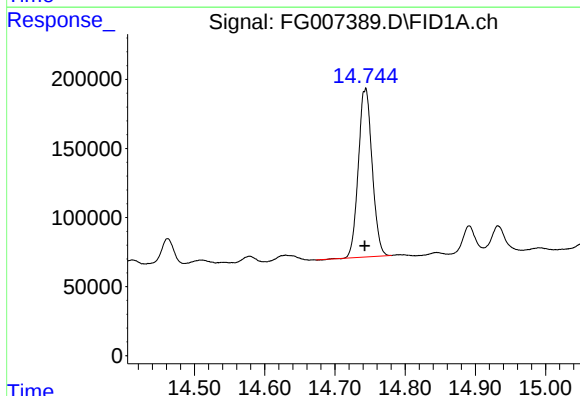


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.743 min
Delta R.T.: 0.001 min
Response: 1666108
Conc: 13.54 ug/ml

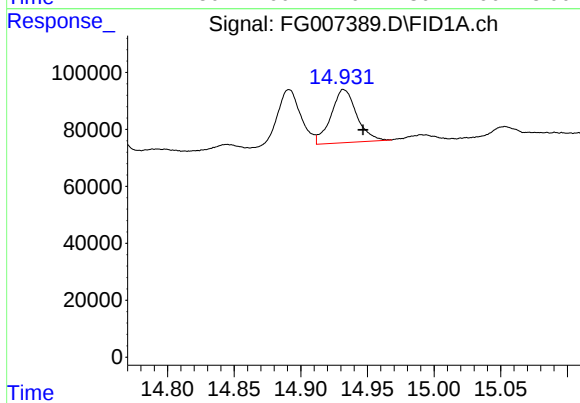

#10 N-TETRACOSANE


R.T.: 14.932 min
Delta R.T.: -0.015 min
Response: 251170
Conc: 1.80 ug/ml

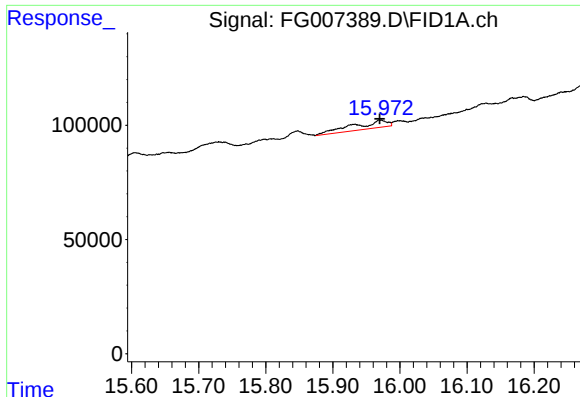

#11 N-HEXACOSANE


R.T.: 15.970 min
Delta R.T.: 0.000 min
Response: 121388
Conc: 0.89 ug/ml

Instrument :
FID_G
ClientSampleId :

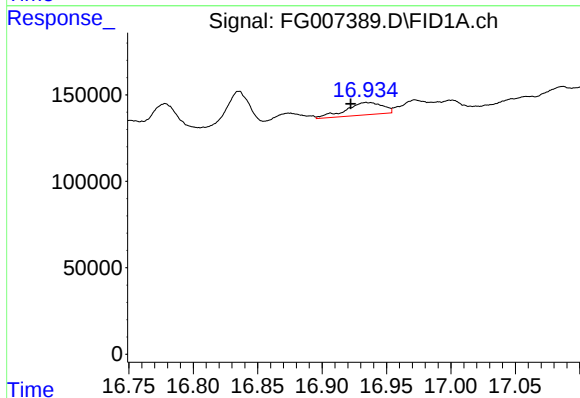


#12 N-OCTACOSANE

R.T.: 16.934 min
Delta R.T.: 0.012 min
Response: 142241
Conc: 1.07 ug/ml

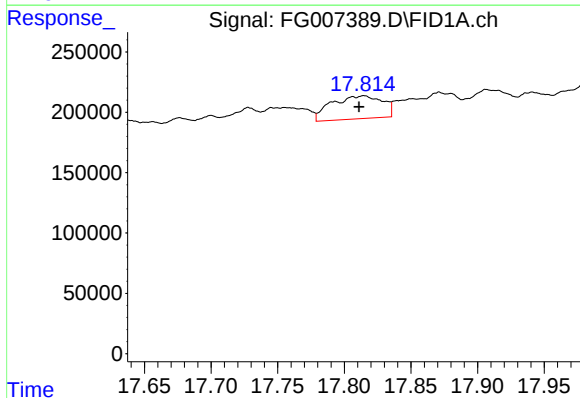


#13 N-TRIACONTANE

R.T.: 17.815 min
Delta R.T.: 0.004 min
Response: 507631
Conc: 3.95 ug/ml

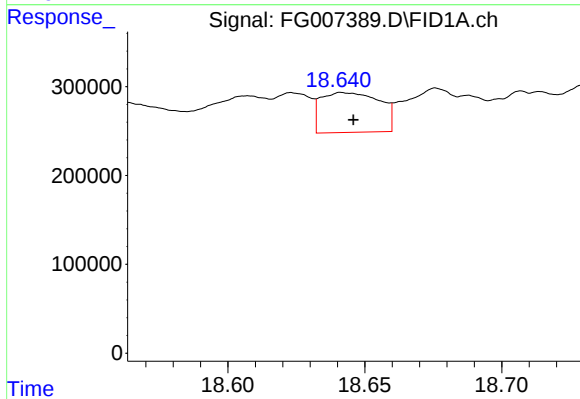

#14 N-DOTRIACONTANE


R.T.: 18.642 min
Delta R.T.: -0.004 min
Response: 669228
Conc: 5.64 ug/ml

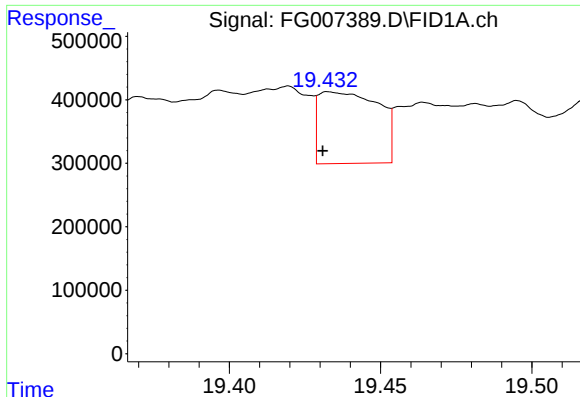

#15 N-TETRATRIACONTANE


R.T.: 19.433 min
Delta R.T.: 0.002 min
Response: 1556540
Conc: 16.11 ug/ml

Instrument :
FID_G
ClientSampleId :

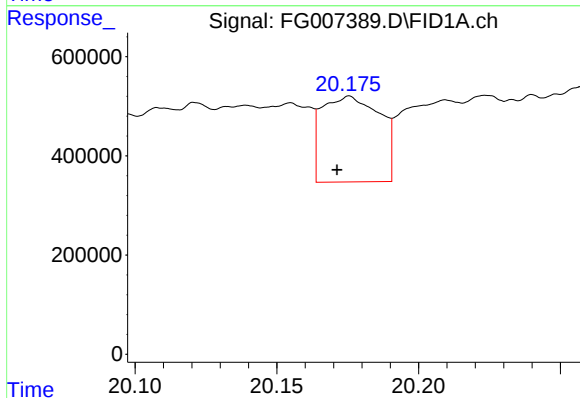


#16 N-HEXATRIACONTANE

R.T.: 20.176 min
Delta R.T.: 0.004 min
Response: 2465599
Conc: 32.06 ug/ml

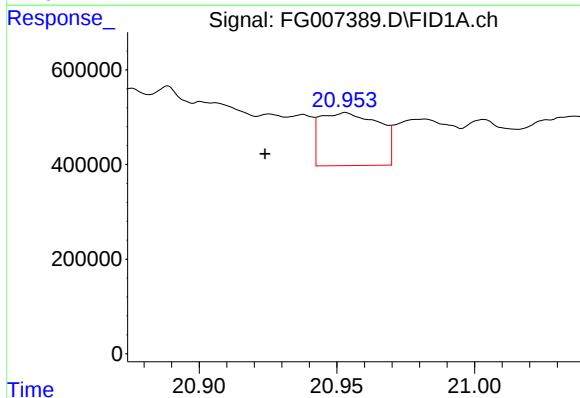

#17 N-OCTATRIACONTANE

R.T.: 20.953 min
Delta R.T.: 0.029 min
Response: 1666402
Conc: 25.27 ug/ml

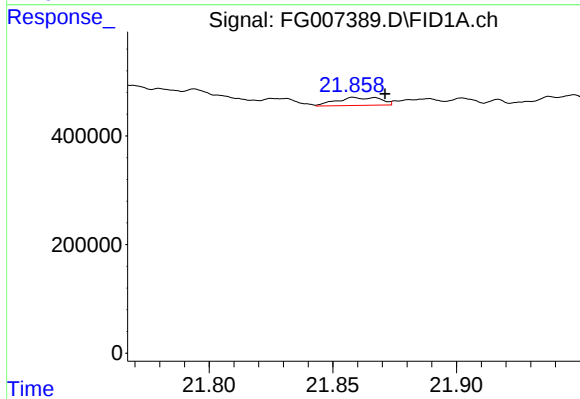

#18 N-TETRACONTANE

R.T.: 21.859 min
Delta R.T.: -0.012 min
Response: 180072
Conc: 2.80 ug/ml