

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112520\
 Data File : FG007387.D
 Signal(s) : FID1A.ch
 Acq On : 25 Nov 2020 13:25
 Operator : DD\AJ
 Sample : L4882-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PAV-B48-112320-0-10

Integration File: autoint1.e
 Quant Time: Nov 26 00:43:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
 Quant Title :
 QLast Update : Tue Nov 03 02:04:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	1689966	13.737 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112520\
Data File : FG007387.D
Signal(s) : FID1A.ch
Acq On : 25 Nov 2020 13:25
Operator : DD\AJ
Sample : L4882-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PAV-B48-112320-0-10

Integration File: autoint1.e
Quant Time: Nov 26 00:43:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

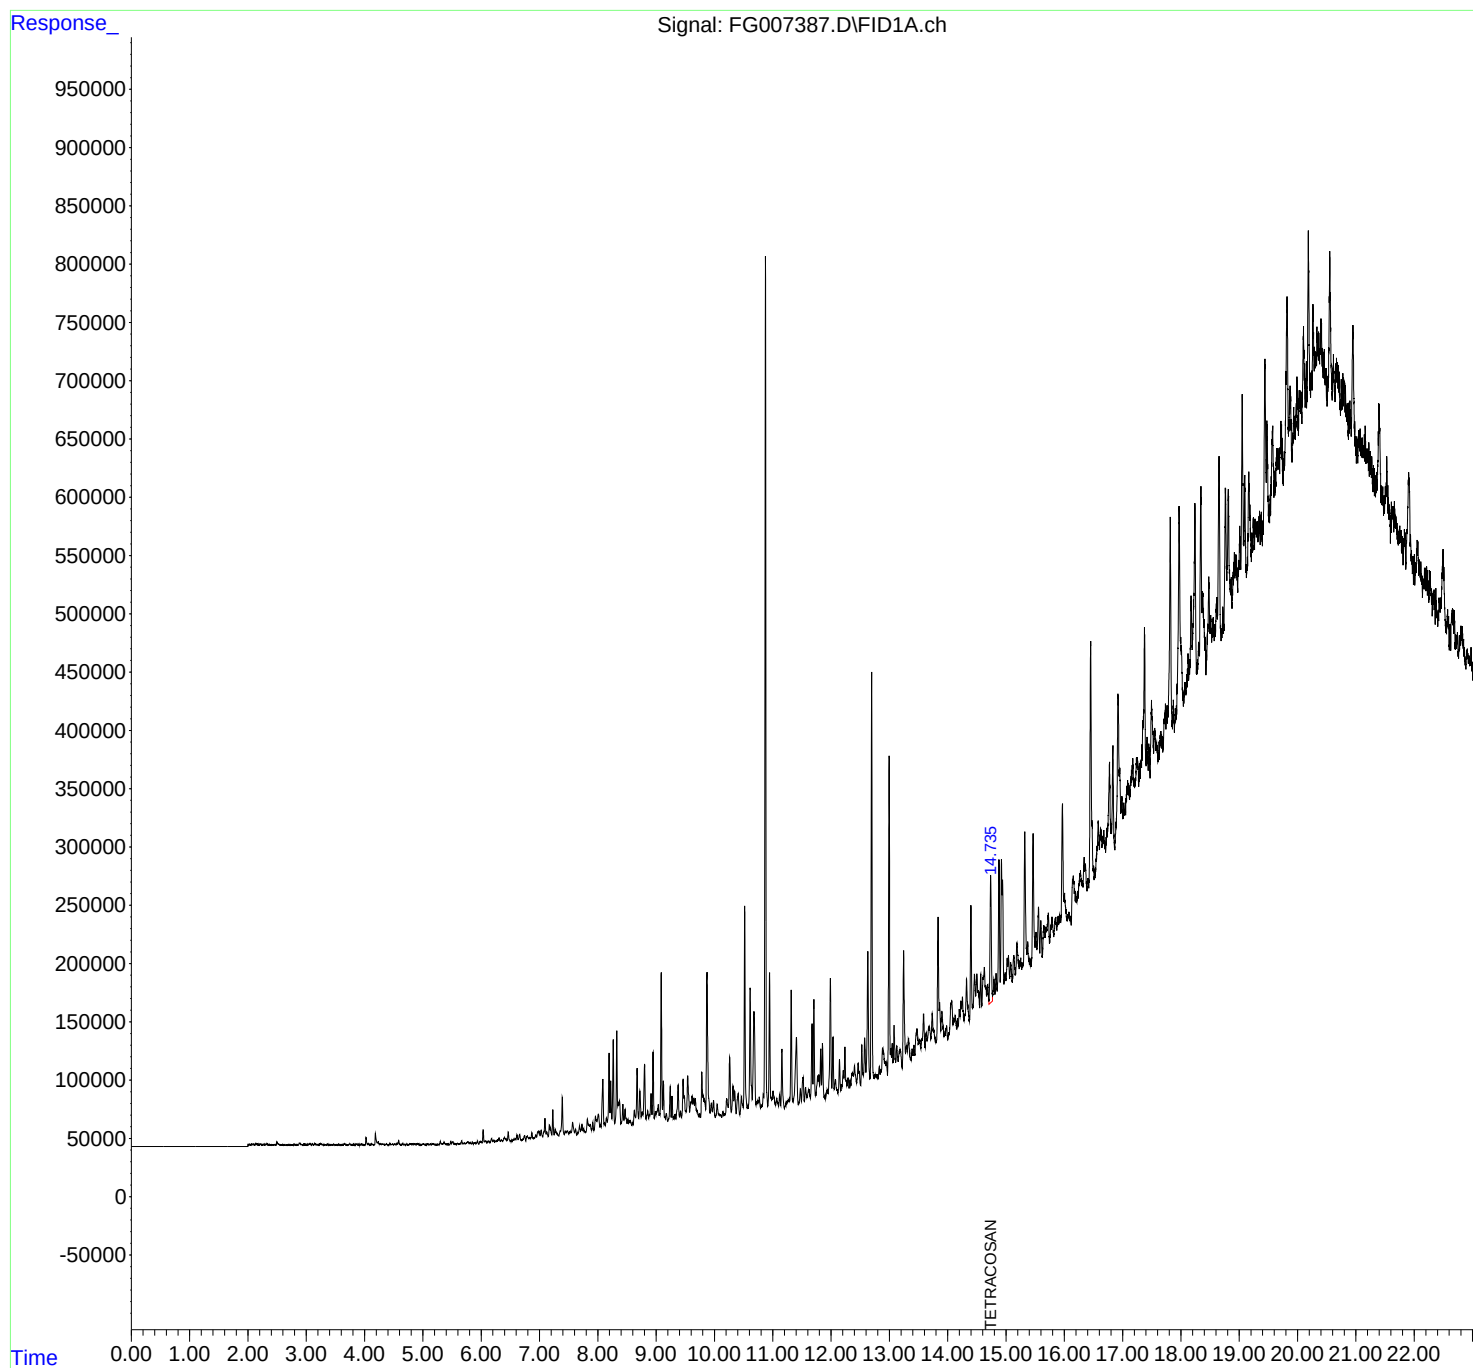

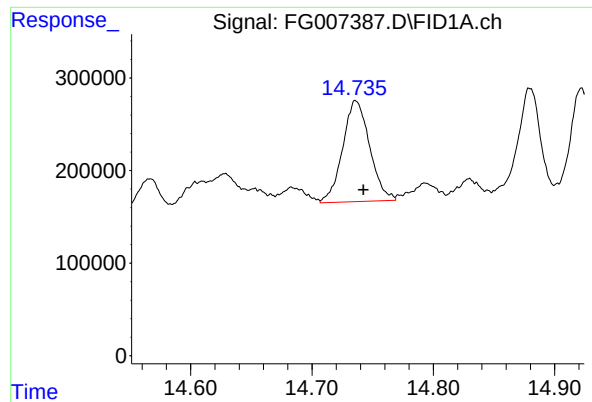

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min
Delta R.T.: -0.006 min
Response: 1689966
Conc: 13.74 ug/ml

Instrument :
FID_G
ClientSampleId :
PAV-B48-112320-0-10