

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112918\
 Data File : FG003080.D
 Signal(s) : FID1A.ch
 Acq On : 29 Nov 2018 13:38
 Operator : AJ\SJ
 Sample : J6062-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 30 06:00:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
 Quant Title :
 QLast Update : Thu Nov 29 04:54:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.713	1714596	15.733 ug/ml
Target Compounds			
4) N-TETRADECANE	8.301f	363579	2.993 ug/ml
5) N-HEXADECANE	9.857	471637	3.803 ug/ml
7) N-EICOSANE	12.586	325301	2.592 ug/ml
8) N-DOCOSANE	13.812	364217	2.912 ug/ml
10) N-TETRACOSANE	14.898	3294789	26.508 ug/ml
11) N-HEXACOSANE	15.947	381290	3.069 ug/ml
12) N-OCTACOSANE	16.905	1308037	10.496 ug/ml
13) N-TRIACONTANE	17.791	783174	6.155 ug/ml
14) N-DOTRIACONTANE	18.626	424965	3.391 ug/ml
16) N-HEXATRIACONTANE	20.134	127524	1.063 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112918\
Data File : FG003080.D
Signal(s) : FID1A.ch
Acq On : 29 Nov 2018 13:38
Operator : AJ\SJ
Sample : J6062-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 30 06:00:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
Quant Title :
QLast Update : Thu Nov 29 04:54:55 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

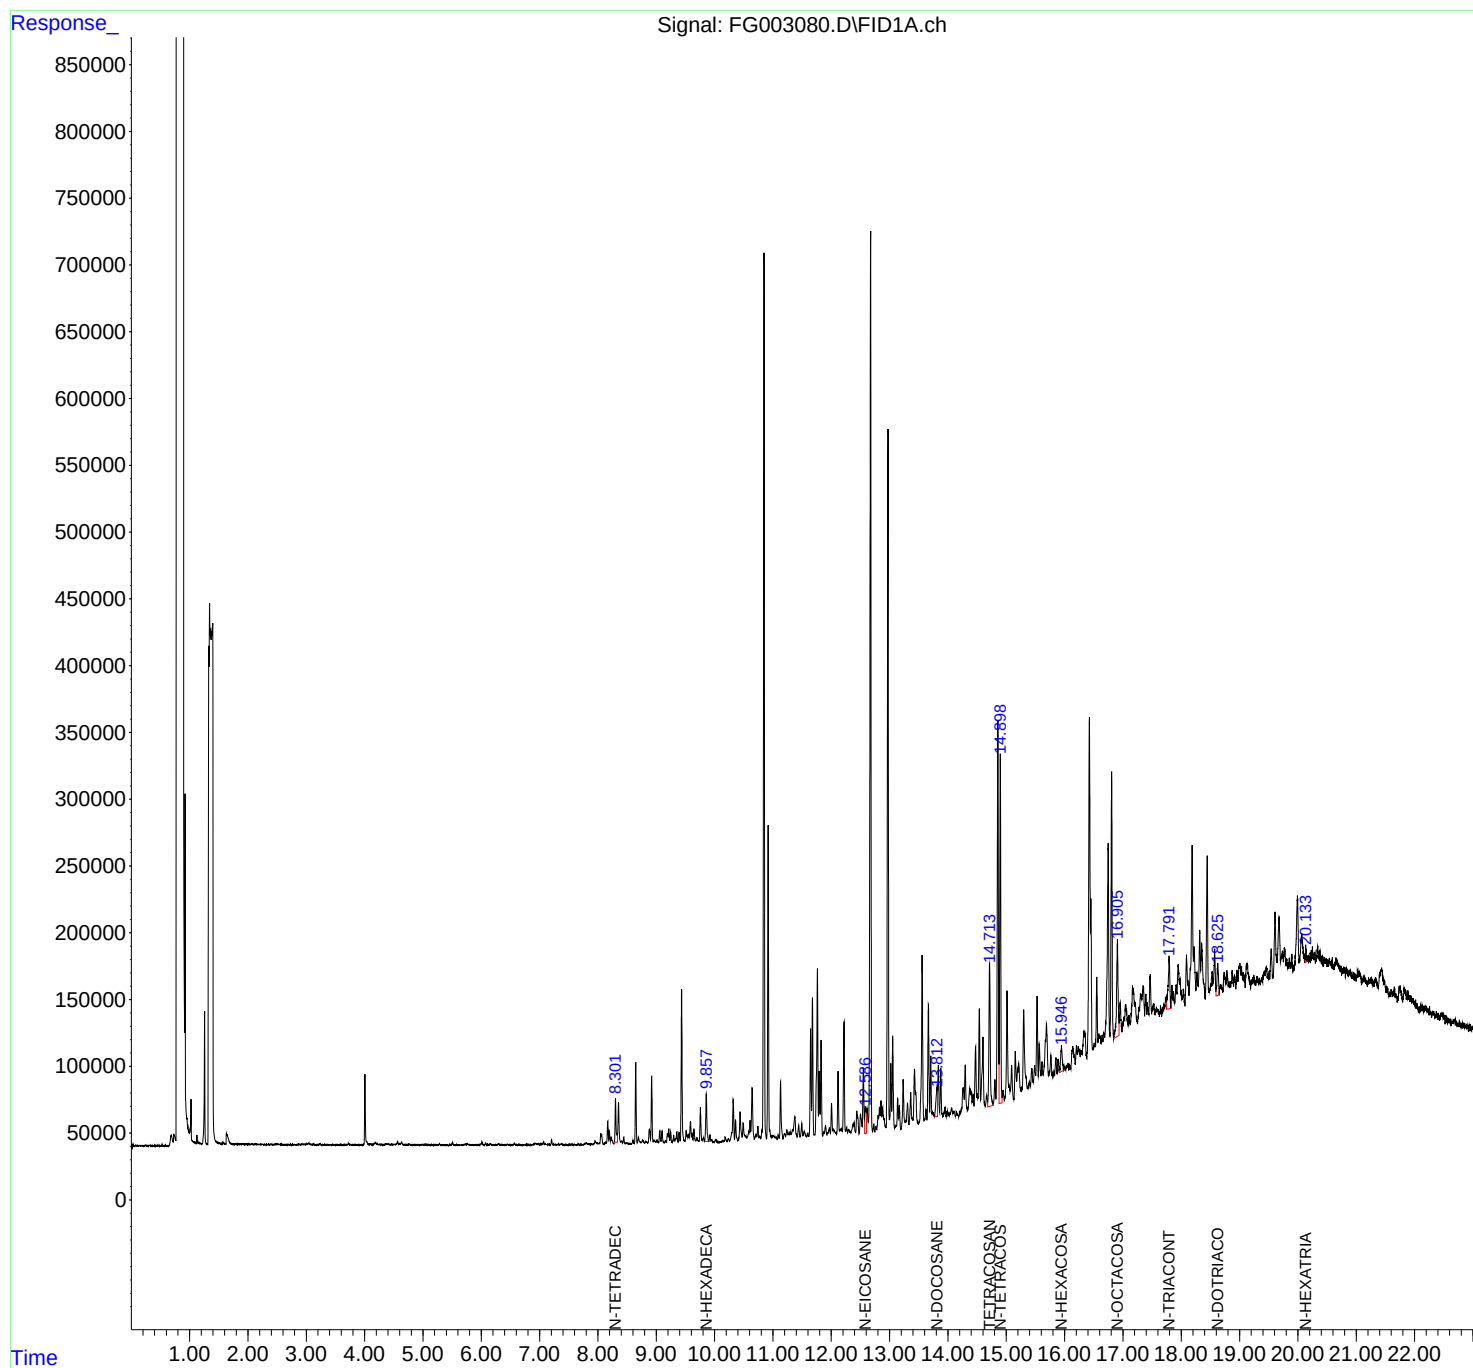

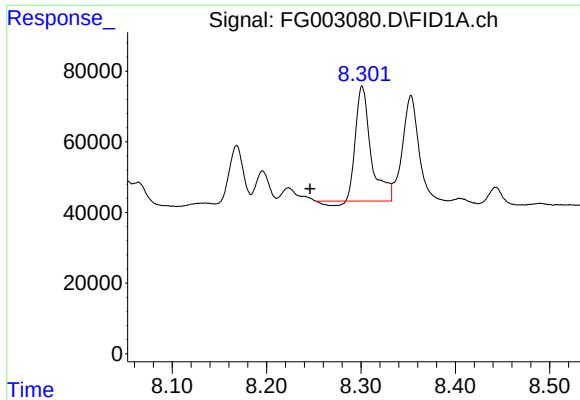


#4 N-TETRADECANE

R.T.: 8.301 min
Delta R.T.: 0.055 min
Response: 363579
Conc: 2.99 ug/ml

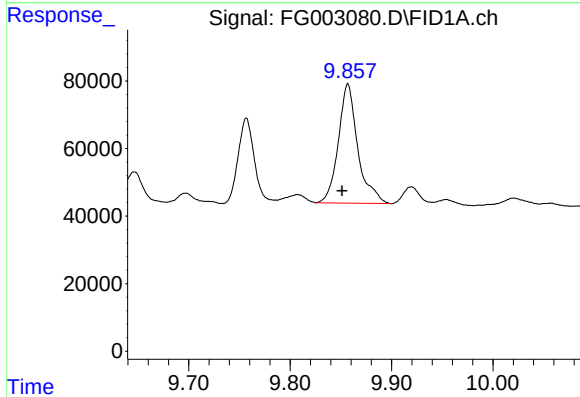


#5 N-HEXADECANE

R.T.: 9.857 min
Delta R.T.: 0.006 min
Response: 471637
Conc: 3.80 ug/ml

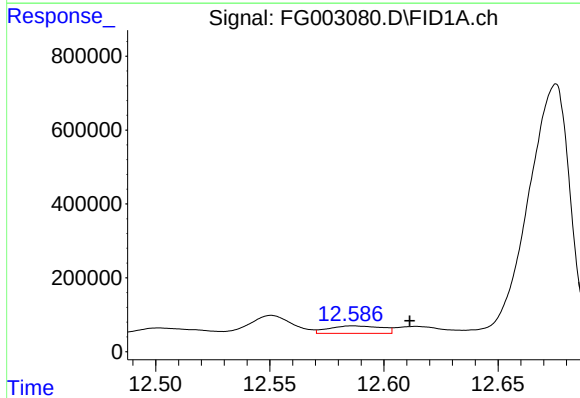


#7 N-EICOSANE

R.T.: 12.586 min
Delta R.T.: -0.025 min
Response: 325301
Conc: 2.59 ug/ml

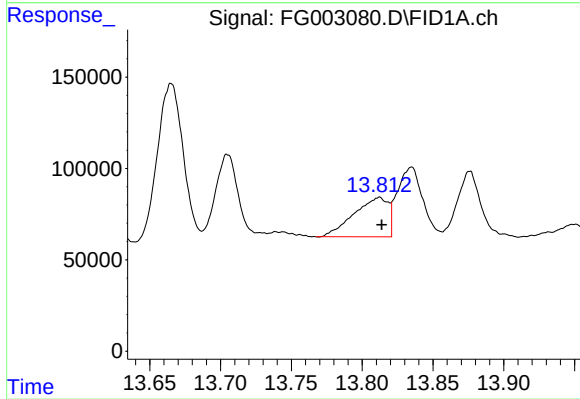


#8 N-DOCOSANE

R.T.: 13.812 min
Delta R.T.: -0.002 min
Response: 364217
Conc: 2.91 ug/ml

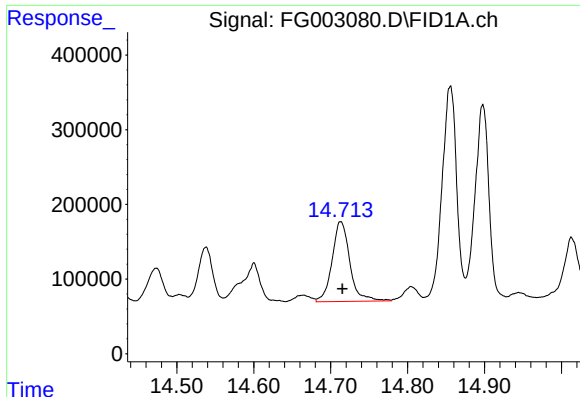


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.713 min
Delta R.T.: -0.002 min
Response: 1714596
Conc: 15.73 ug/ml

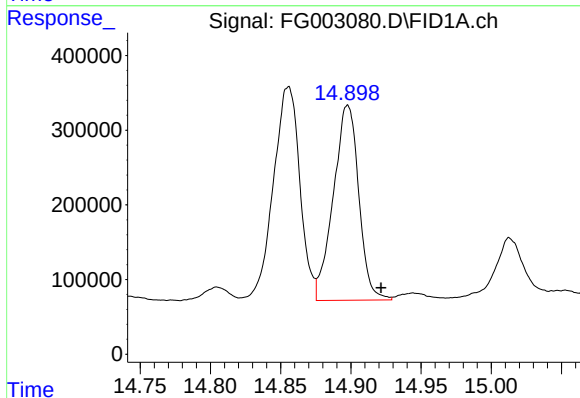


#10 N-TETRACOSANE

R.T.: 14.898 min
Delta R.T.: -0.024 min
Response: 3294789
Conc: 26.51 ug/ml

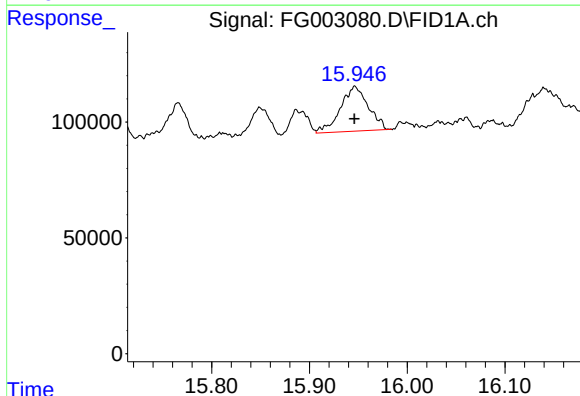


#11 N-HEXACOSANE

R.T.: 15.947 min
Delta R.T.: 0.000 min
Response: 381290
Conc: 3.07 ug/ml

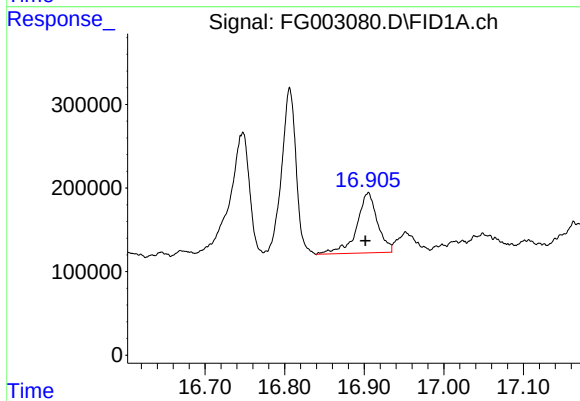


#12 N-OCTACOSANE

R.T.: 16.905 min
Delta R.T.: 0.004 min
Response: 1308037
Conc: 10.50 ug/ml

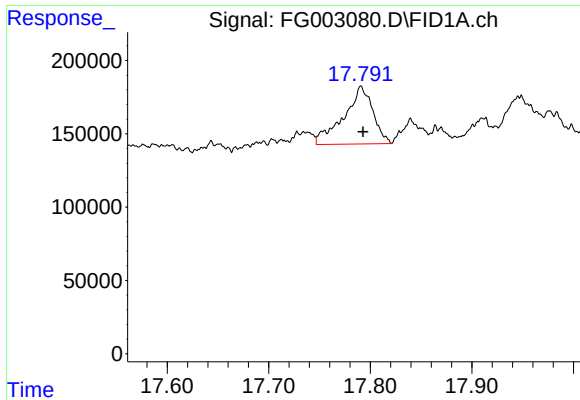


#13 N-TRIACONTANE

R.T.: 17.791 min
Delta R.T.: -0.002 min
Response: 783174
Conc: 6.15 ug/ml

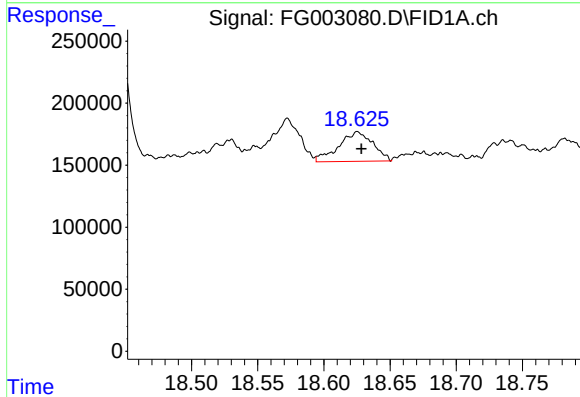

#14 N-DOTRIACONTANE

R.T.: 18.626 min
Delta R.T.: -0.003 min
Response: 424965
Conc: 3.39 ug/ml

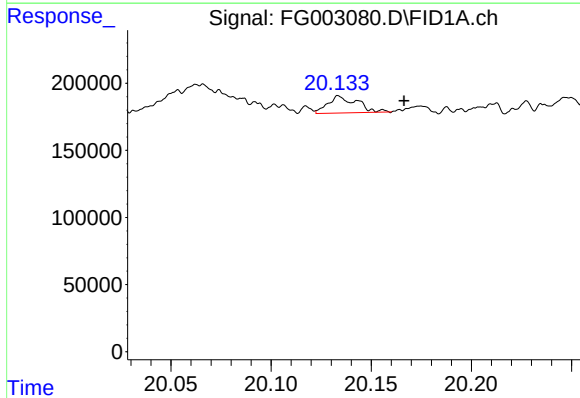

#16 N-HEXATRIACONTANE

R.T.: 20.134 min
Delta R.T.: -0.032 min
Response: 127524
Conc: 1.06 ug/ml