

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112918\
 Data File : FG003088.D
 Signal(s) : FID1A.ch
 Acq On : 29 Nov 2018 17:40
 Operator : AJ\SJ
 Sample : J6062-02 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 30 06:02:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
 Quant Title :
 QLast Update : Thu Nov 29 04:54:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.714	777861	7.138 ug/ml
Target Compounds			
4) N-TETRADECANE	8.303f	190801	1.570 ug/ml
5) N-HEXADECANE	9.860	222022	1.790 ug/ml
7) N-EICOSANE	12.554f	210997	1.681 ug/ml
8) N-DOCOSANE	13.839	225292	1.802 ug/ml
10) N-TETRACOSANE	14.899	1466386	11.798 ug/ml
12) N-OCTACOSANE	16.905	469858	3.770 ug/ml
13) N-TRIACONTANE	17.791	309497	2.432 ug/ml
14) N-DOTRIACONTANE	18.628	168165	1.342 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112918\
Data File : FG003088.D
Signal(s) : FID1A.ch
Acq On : 29 Nov 2018 17:40
Operator : AJ\SJ
Sample : J6062-02 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 30 06:02:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
Quant Title :
QLast Update : Thu Nov 29 04:54:55 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

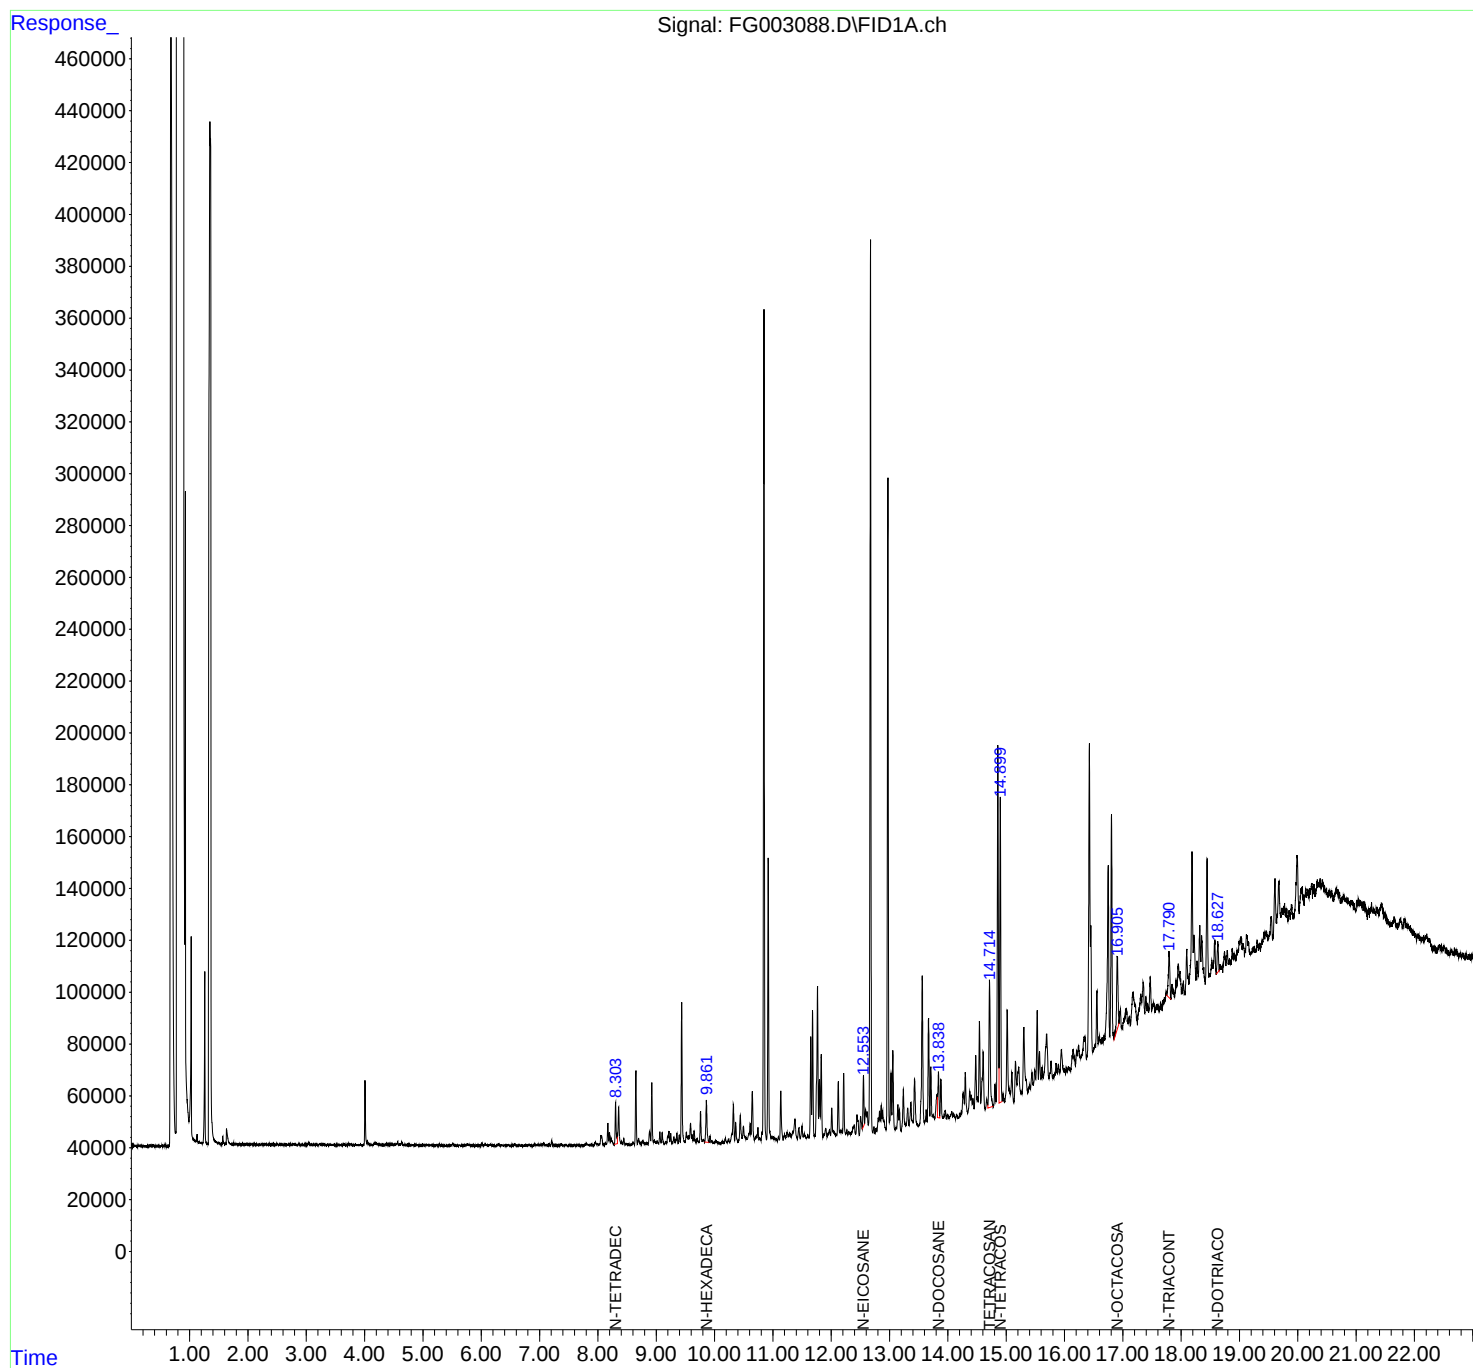

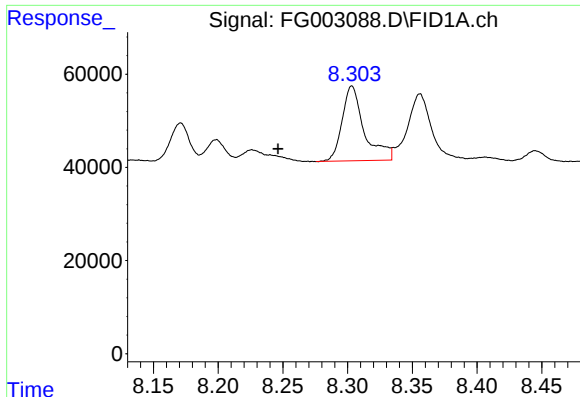


#4 N-TETRADECANE

R.T.: 8.303 min
Delta R.T.: 0.057 min
Response: 190801
Conc: 1.57 ug/ml

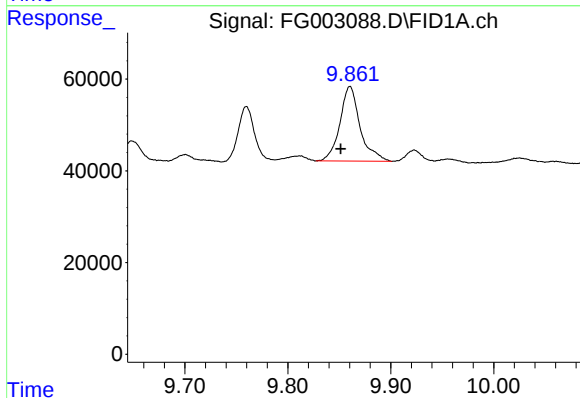


#5 N-HEXADECANE

R.T.: 9.860 min
Delta R.T.: 0.009 min
Response: 222022
Conc: 1.79 ug/ml

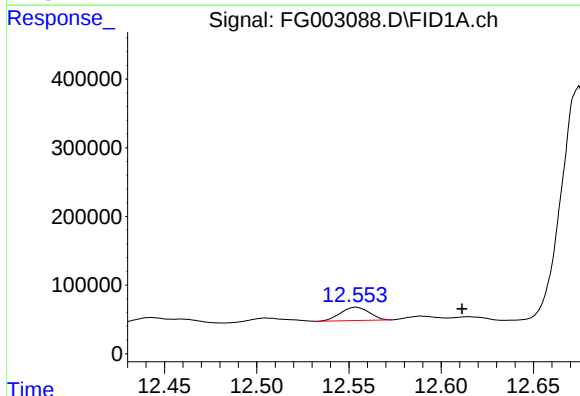


#7 N-EICOSANE

R.T.: 12.554 min
Delta R.T.: -0.058 min
Response: 210997
Conc: 1.68 ug/ml

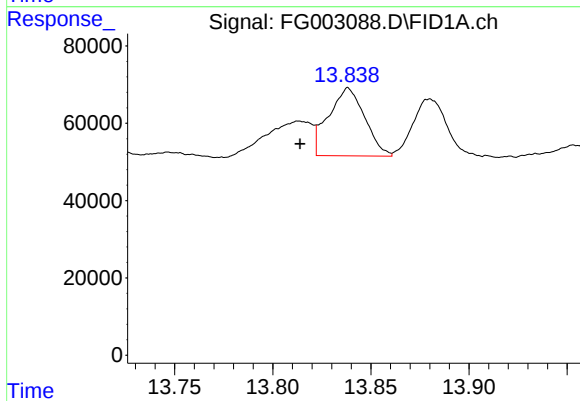


#8 N-DOCOSANE

R.T.: 13.839 min
Delta R.T.: 0.025 min
Response: 225292
Conc: 1.80 ug/ml

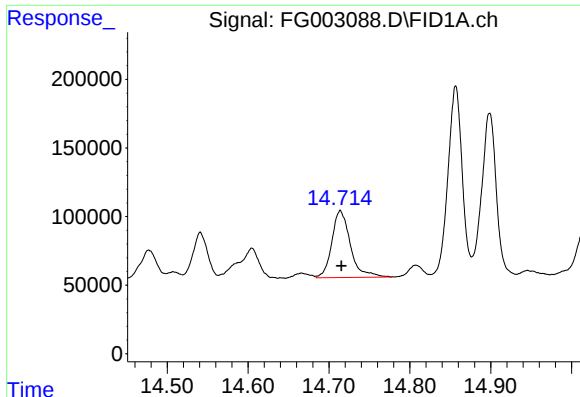


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.714 min
Delta R.T.: -0.001 min
Response: 777861
Conc: 7.14 ug/ml

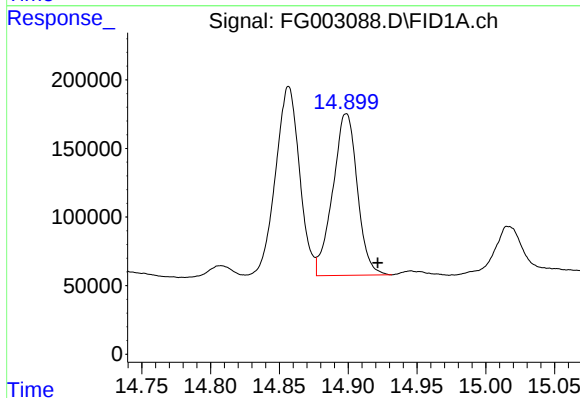


#10 N-TETRACOSANE

R.T.: 14.899 min
Delta R.T.: -0.023 min
Response: 1466386
Conc: 11.80 ug/ml

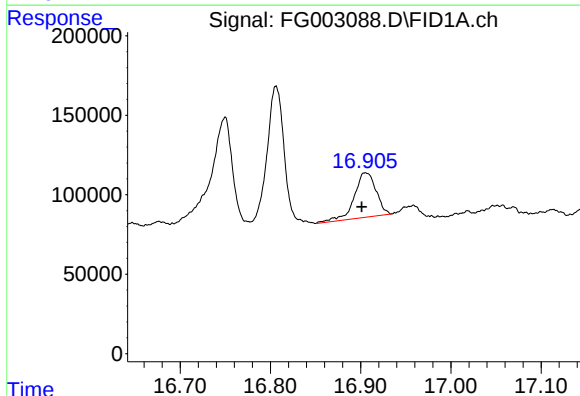


#12 N-OCTACOSANE

R.T.: 16.905 min
Delta R.T.: 0.004 min
Response: 469858
Conc: 3.77 ug/ml

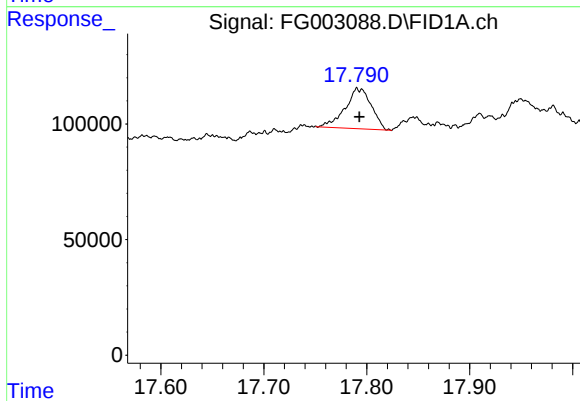

#13 N-TRIACONTANE

R.T.: 17.791 min
Delta R.T.: -0.002 min
Response: 309497
Conc: 2.43 ug/ml

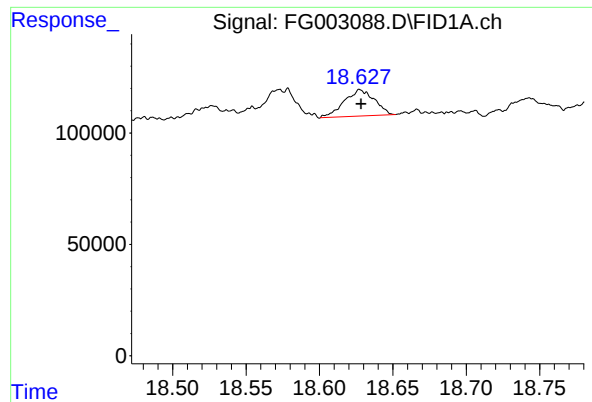

#14 N-DOTRIACONTANE

R.T.: 18.628 min
Delta R.T.: 0.000 min
Response: 168165
Conc: 1.34 ug/ml