

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112918\
 Data File : FG003078.D
 Signal(s) : FID1A.ch
 Acq On : 29 Nov 2018 12:37
 Operator : AJ\SJ
 Sample : PB115158BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 30 06:00:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
 Quant Title :
 QLast Update : Thu Nov 29 04:54:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	1785776	16.386 ug/ml
Target Compounds			
2) N-DECANE	4.418	2005551	17.163 ug/ml
3) N-DODECANE	6.443	2099879	17.653 ug/ml
4) N-TETRADECANE	8.243	2140522	17.618 ug/ml
5) N-HEXADECANE	9.847	2175128	17.540 ug/ml
6) N-OCTADECANE	11.292	2188790	17.412 ug/ml
7) N-EICOSANE	12.606	2185480	17.416 ug/ml
8) N-DOCOSANE	13.809	2177964	17.416 ug/ml
10) N-TETRACOSANE	14.915	2167795	17.441 ug/ml
11) N-HEXACOSANE	15.942	2144388	17.259 ug/ml
12) N-OCTACOSANE	16.896	2134013	17.124 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112918\
Data File : FG003078.D
Signal(s) : FID1A.ch
Acq On : 29 Nov 2018 12:37
Operator : AJ\SJ
Sample : PB115158BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 30 06:00:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
Quant Title :
QLast Update : Thu Nov 29 04:54:55 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

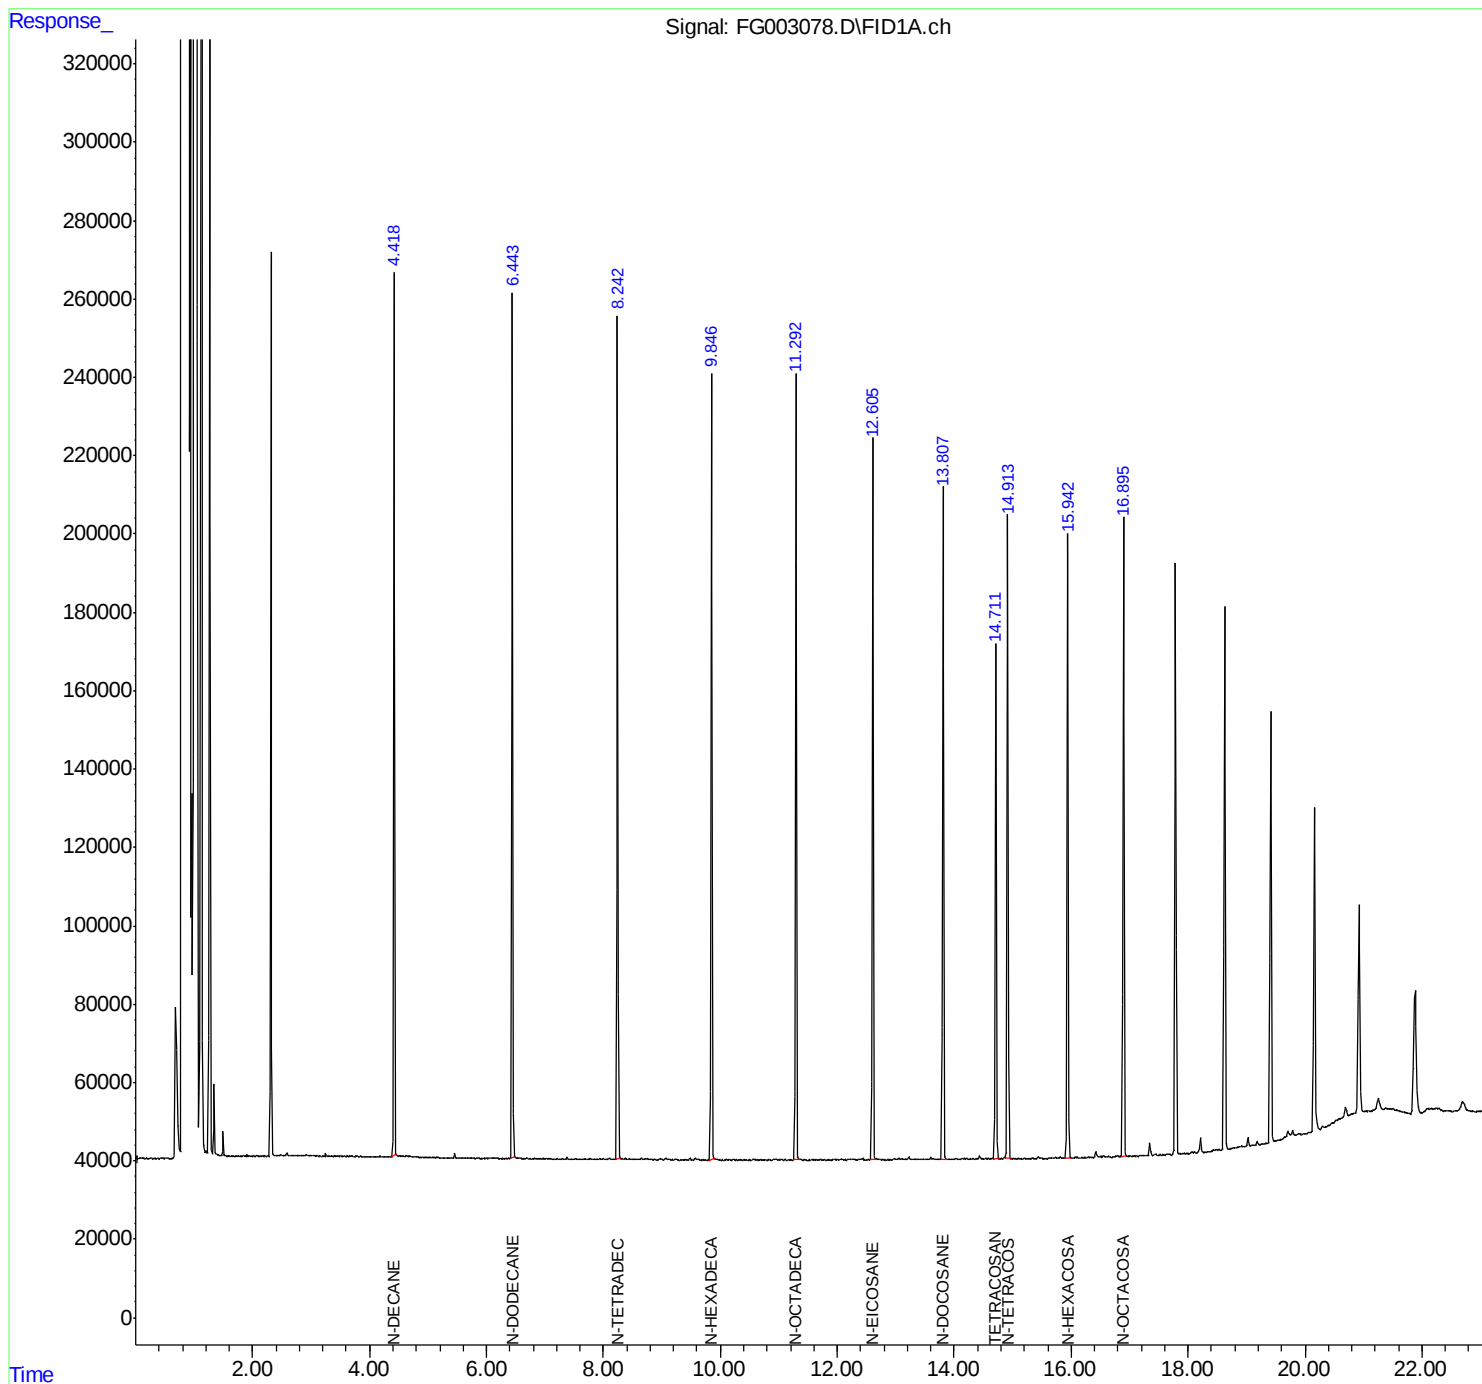

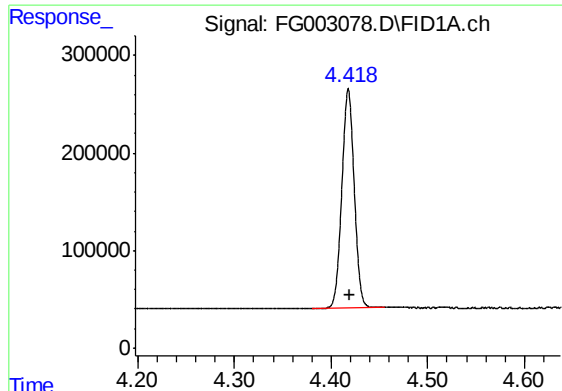


#2 N-DECANE

R.T.: 4.418 min
Delta R.T.: -0.001 min
Response: 2005551
Conc: 17.16 ug/ml

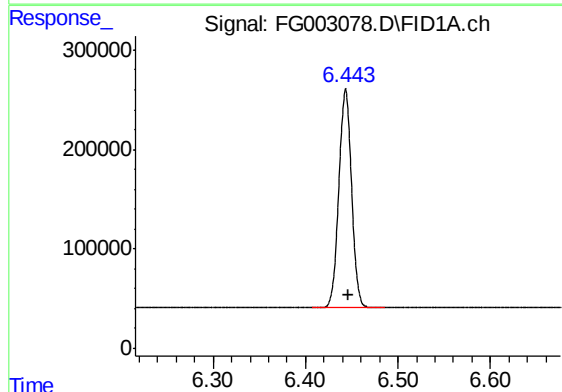


#3 N-DODECANE

R.T.: 6.443 min
Delta R.T.: -0.003 min
Response: 2099879
Conc: 17.65 ug/ml

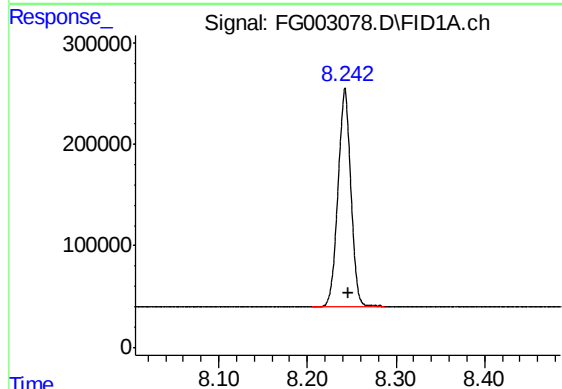


#4 N-TETRADECANE

R.T.: 8.243 min
Delta R.T.: -0.004 min
Response: 2140522
Conc: 17.62 ug/ml

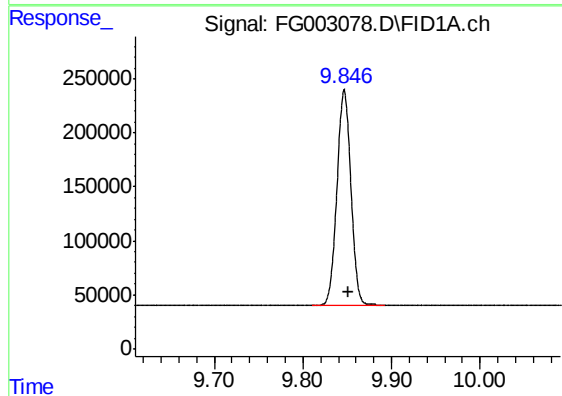


#5 N-HEXADECANE

R.T.: 9.847 min
Delta R.T.: -0.005 min
Response: 2175128
Conc: 17.54 ug/ml

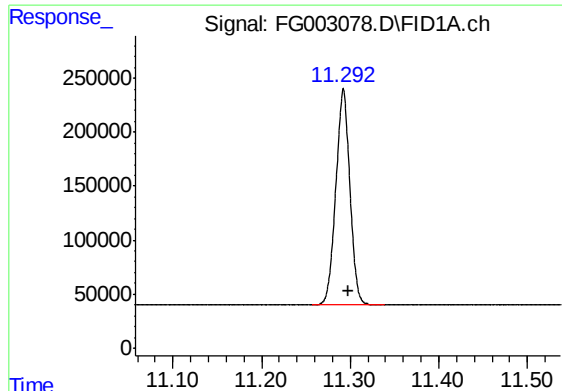


#6 N-OCTADECANE

R.T.: 11.292 min
Delta R.T.: -0.005 min
Response: 2188790
Conc: 17.41 ug/ml

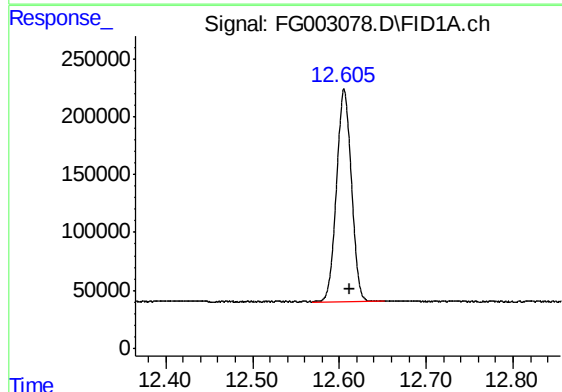


#7 N-EICOSANE

R.T.: 12.606 min
Delta R.T.: -0.006 min
Response: 2185480
Conc: 17.42 ug/ml

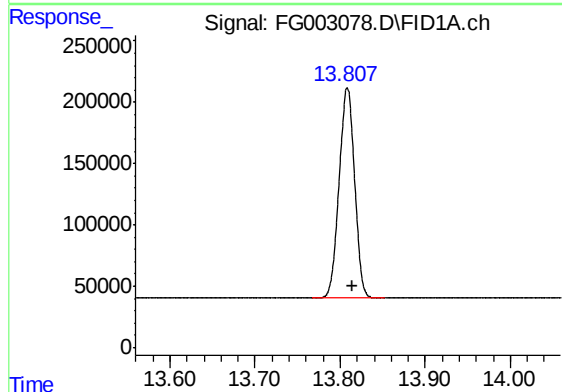


#8 N-DOCOSANE

R.T.: 13.809 min
Delta R.T.: -0.005 min
Response: 2177964
Conc: 17.42 ug/ml

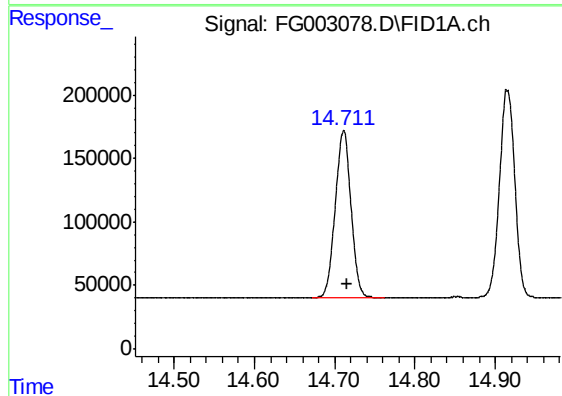


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.711 min
Delta R.T.: -0.004 min
Response: 1785776
Conc: 16.39 ug/ml

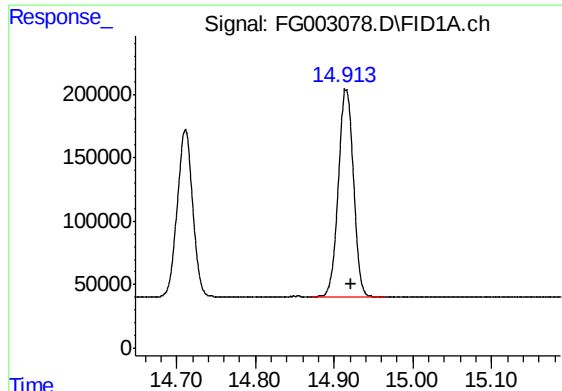


#10 N-TETRACOSANE

R.T.: 14.915 min
Delta R.T.: -0.007 min
Response: 2167795
Conc: 17.44 ug/ml

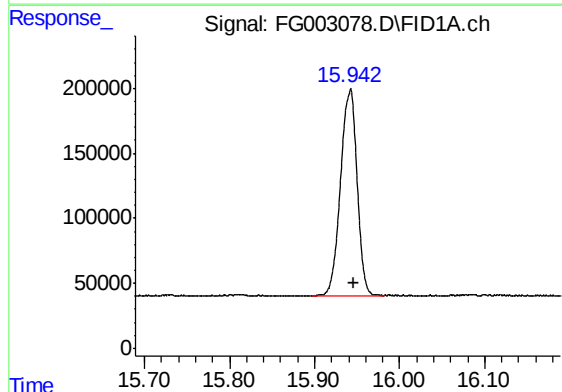

#11 N-HEXACOSANE

R.T.: 15.942 min
Delta R.T.: -0.004 min
Response: 2144388
Conc: 17.26 ug/ml

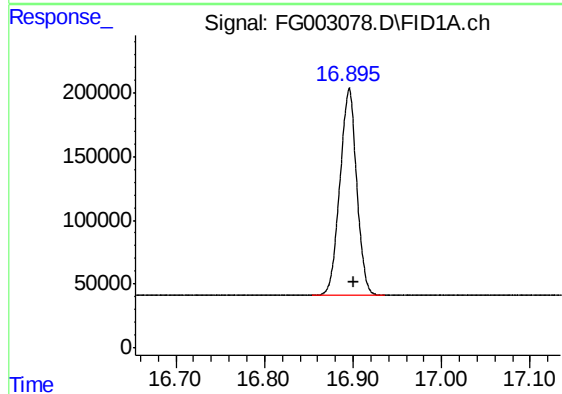

#12 N-OCTACOSANE

R.T.: 16.896 min
Delta R.T.: -0.006 min
Response: 2134013
Conc: 17.12 ug/ml