

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112918\
 Data File : FG003087.D
 Signal(s) : FID1A.ch
 Acq On : 29 Nov 2018 17:10
 Operator : AJ\SJ
 Sample : J5767-17MSD 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 30 06:02:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
 Quant Title :
 QLast Update : Thu Nov 29 04:54:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.713	223640	2.052 ug/ml
Target Compounds			
2) N-DECANE	4.418	179903	1.540 ug/ml
3) N-DODECANE	6.444	191907	1.613 ug/ml
4) N-TETRADECANE	8.243	199722	1.644 ug/mlm
5) N-HEXADECANE	9.848	207007	1.669 ug/ml
6) N-OCTADECANE	11.293	196740	1.565 ug/ml
7) N-EICOSANE	12.607	214794	1.712 ug/ml
8) N-DOCOSANE	13.810	250670	2.004 ug/ml
10) N-TETRACOSANE	14.916	180192	1.450 ug/mlm
11) N-HEXACOSANE	15.944	297508	2.394 ug/ml
12) N-OCTACOSANE	16.899	469168	3.765 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112918\
Data File : FG003087.D
Signal(s) : FID1A.ch
Acq On : 29 Nov 2018 17:10
Operator : AJ\SJ
Sample : J5767-17MSD 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 30 06:02:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
Quant Title :
QLast Update : Thu Nov 29 04:54:55 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

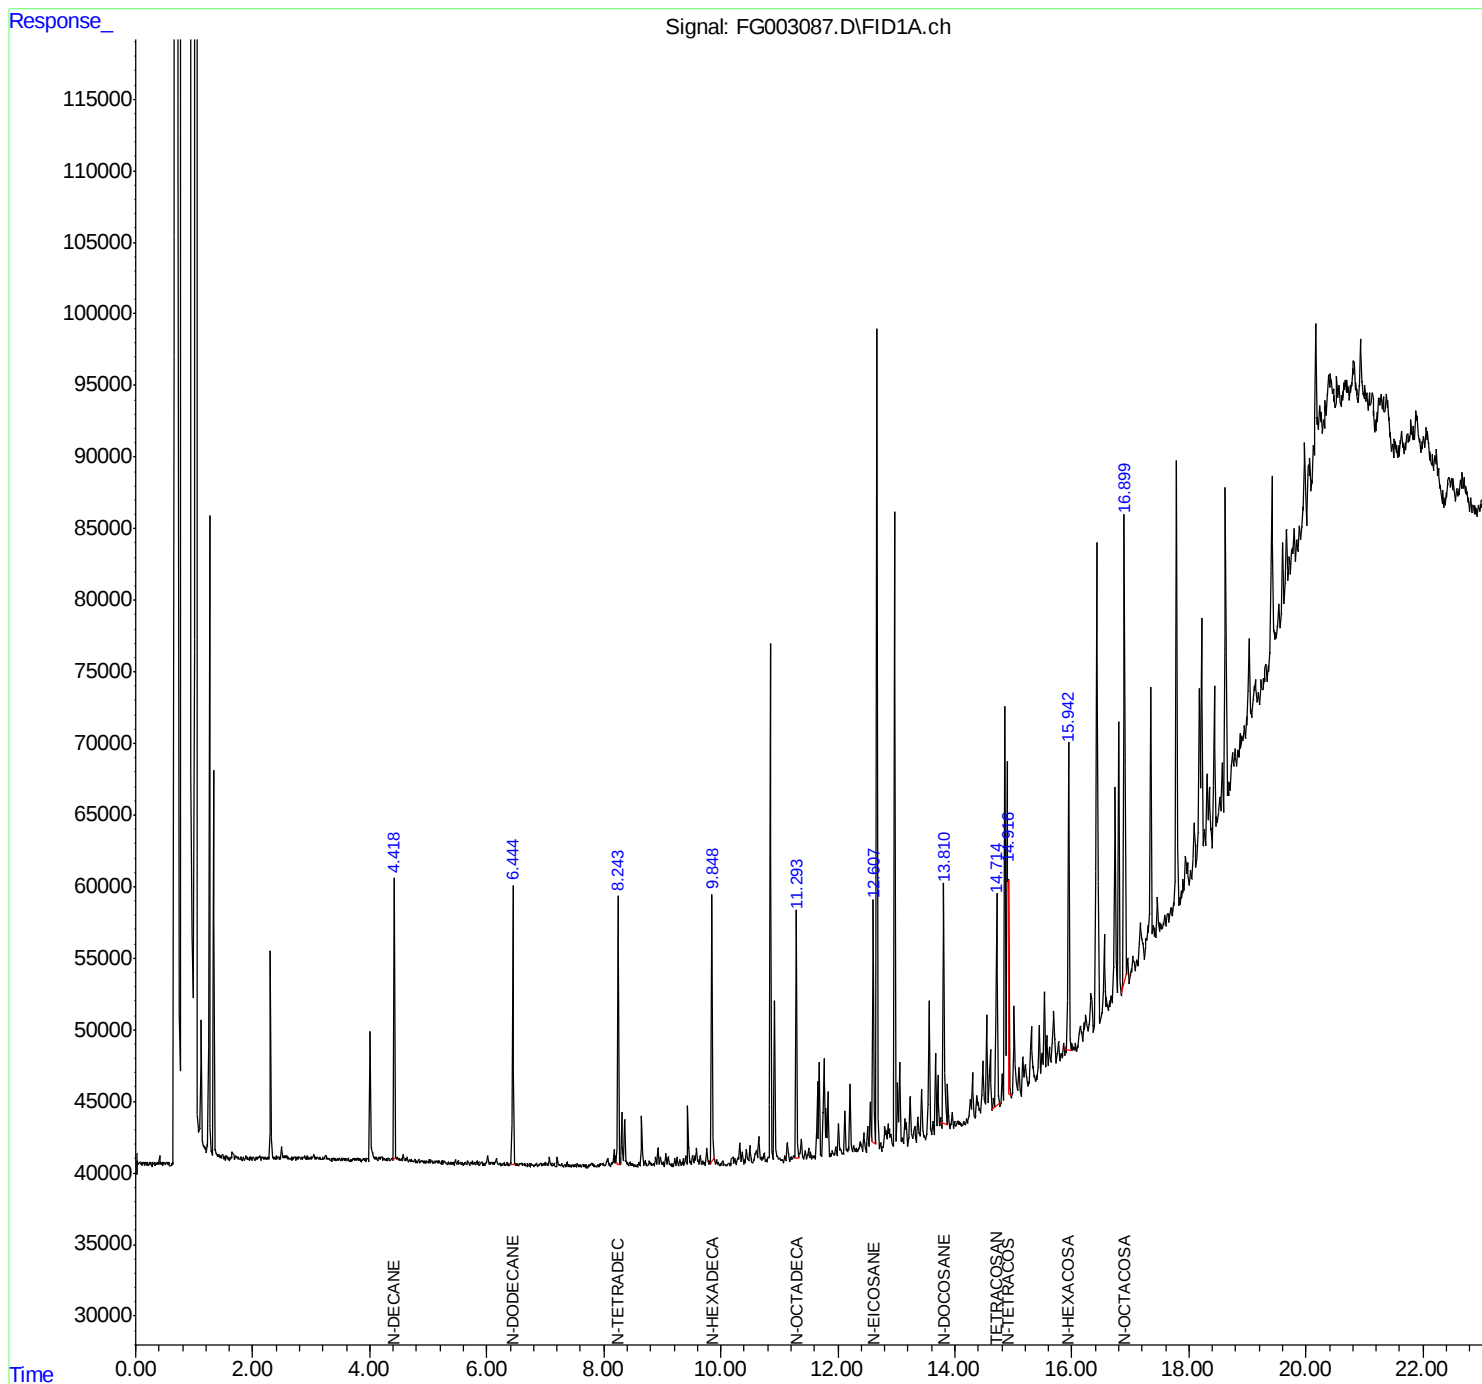

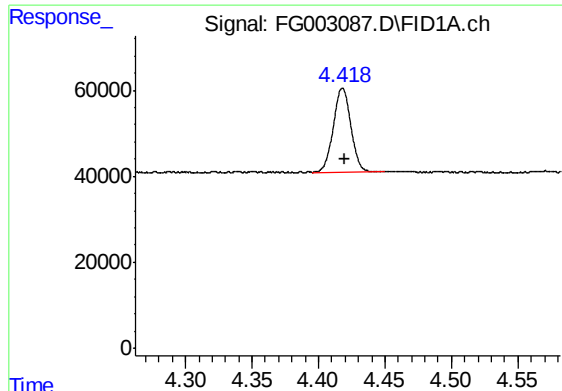


#2 N-DECANE

R.T.: 4.418 min
Delta R.T.: -0.001 min
Response: 179903
Conc: 1.54 ug/ml

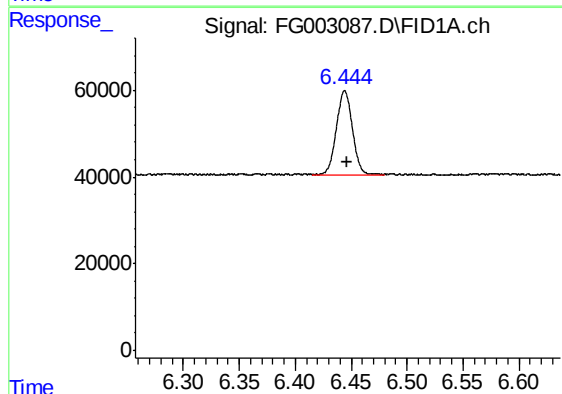


#3 N-DODECANE

R.T.: 6.444 min
Delta R.T.: -0.002 min
Response: 191907
Conc: 1.61 ug/ml

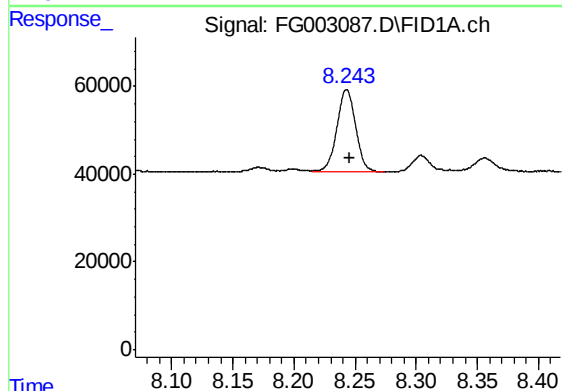


#4 N-TETRADECANE

R.T.: 8.243 min
Delta R.T.: -0.003 min
Response: 199722
Conc: 1.64 ug/ml m

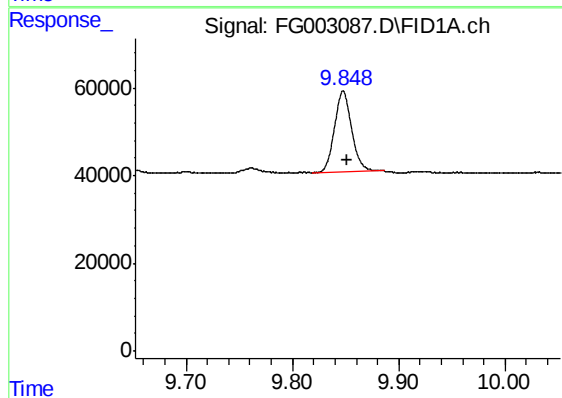


#5 N-HEXADECANE

R.T.: 9.848 min
Delta R.T.: -0.004 min
Response: 207007
Conc: 1.67 ug/ml

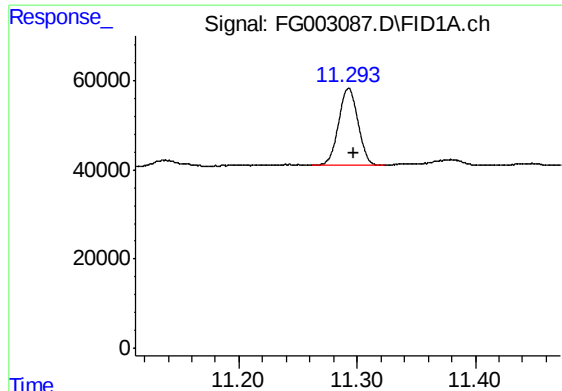


#6 N-OCTADECANE

R.T.: 11.293 min
Delta R.T.: -0.005 min
Response: 196740
Conc: 1.57 ug/ml

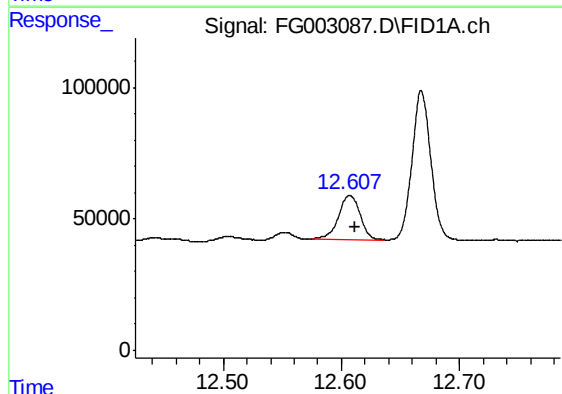


#7 N-EICOSANE

R.T.: 12.607 min
Delta R.T.: -0.004 min
Response: 214794
Conc: 1.71 ug/ml

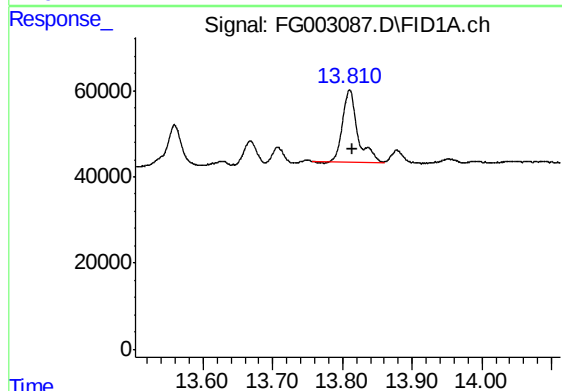


#8 N-DOCOSANE

R.T.: 13.810 min
Delta R.T.: -0.004 min
Response: 250670
Conc: 2.00 ug/ml

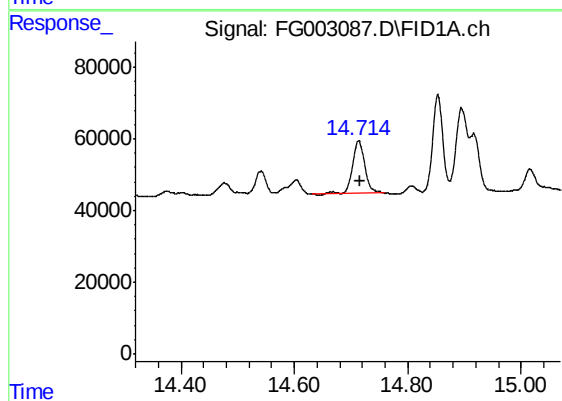


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.713 min
Delta R.T.: -0.002 min
Response: 223640
Conc: 2.05 ug/ml

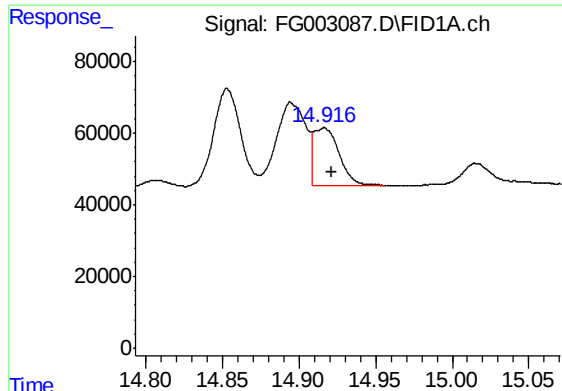


#10 N-TETRACOSANE

R.T.: 14.916 min
Delta R.T.: -0.005 min
Response: 180192
Conc: 1.45 ug/ml m

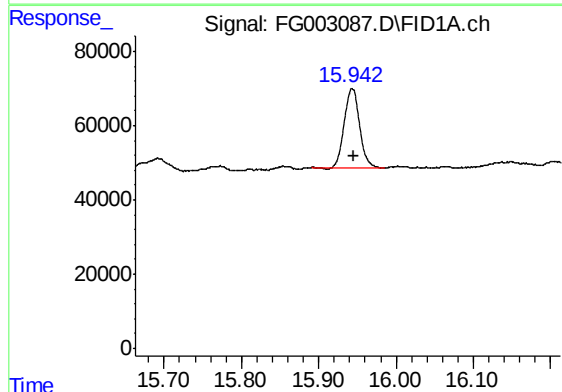

#11 N-HEXACOSANE

R.T.: 15.944 min
Delta R.T.: -0.002 min
Response: 297508
Conc: 2.39 ug/ml

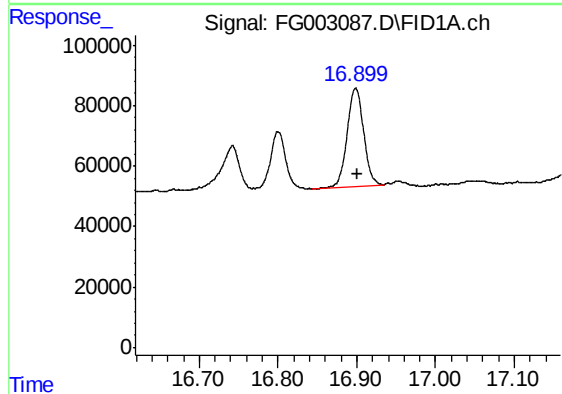

#12 N-OCTACOSANE

R.T.: 16.899 min
Delta R.T.: -0.003 min
Response: 469168
Conc: 3.76 ug/ml