

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120121\
 Data File : FG009118.D
 Signal(s) : FID1A.ch
 Acq On : 01 Dec 2021 16:10
 Operator : AJ\MA
 Sample : M4863-02 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 02 00:07:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
 Quant Title :
 QLast Update : Wed Nov 24 00:59:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.754	374181	3.208 ug/ml
Target Compounds			
7) N-EICOSANE	12.636	117444	0.821 ug/ml
8) N-DOCOSANE	13.893	288961	2.106 ug/ml
10) N-TETRACOSANE	14.956	1160673	8.819 ug/ml
11) N-HEXACOSANE	15.989	127432	1.040 ug/ml
12) N-OCTACOSANE	16.976	276023	2.421 ug/ml
13) N-TRIACONTANE	17.833	149790	1.385 ug/ml
14) N-DOTRIACONTANE	18.661	447683	4.354 ug/ml
15) N-TETRATRIACONTANE	19.457	117725	1.190 ug/ml
16) N-HEXATRIACONTANE	20.204	389919	4.149 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120121\
Data File : FG009118.D
Signal(s) : FID1A.ch
Acq On : 01 Dec 2021 16:10
Operator : AJ\MA
Sample : M4863-02 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 02 00:07:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

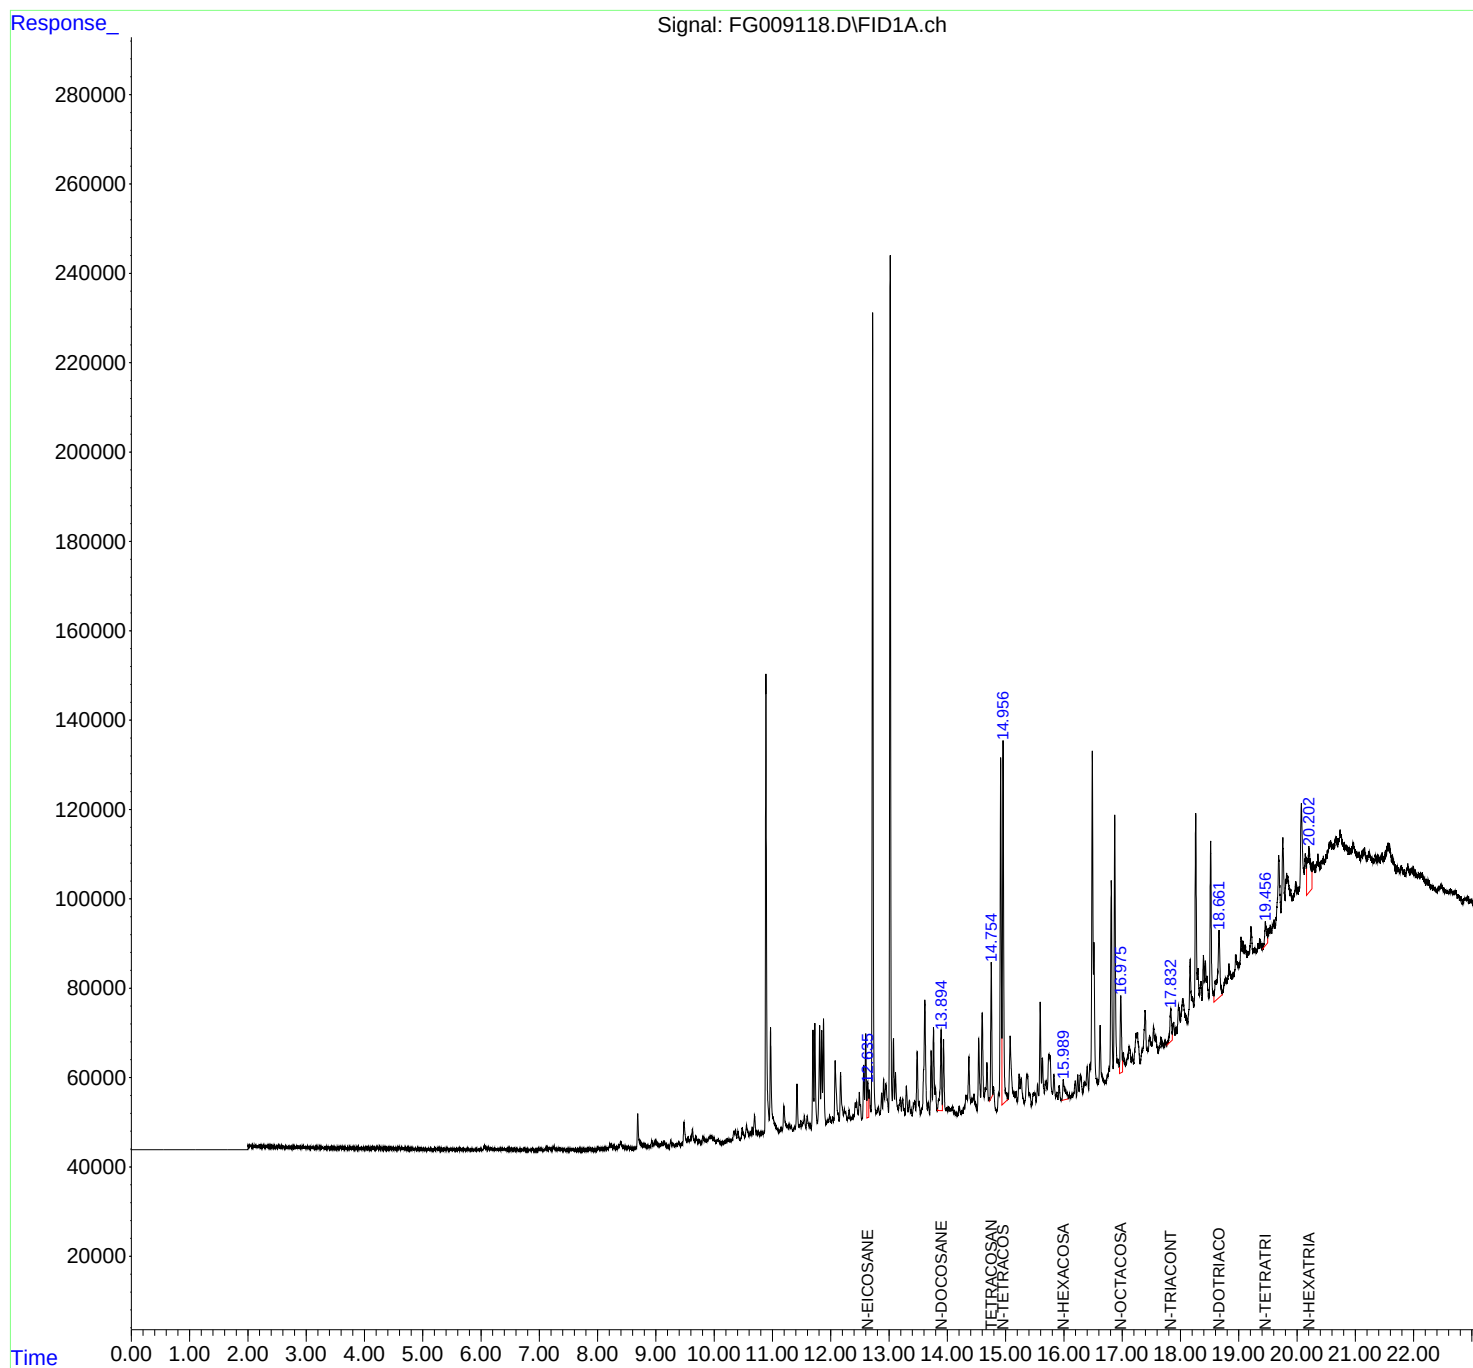


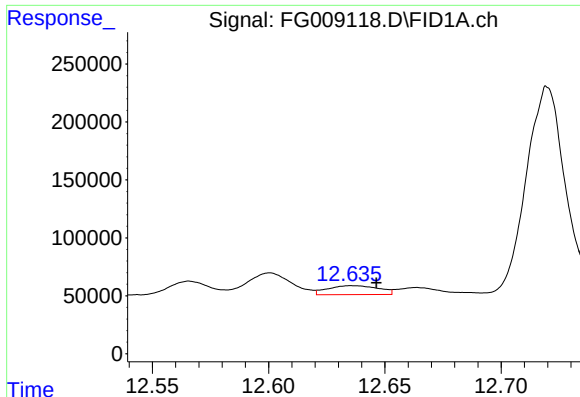

#7 N-EICOSANE


R.T.: 12.636 min
Delta R.T.: -0.010 min
Response: 117444
Conc: 0.82 ug/ml

Instrument :
FID_G
ClientSampleId :

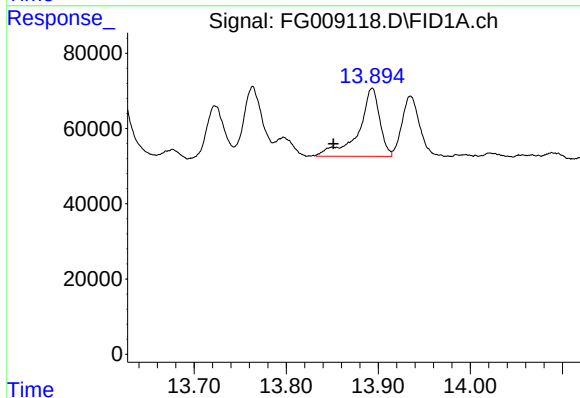


#8 N-DOCOSANE

R.T.: 13.893 min
Delta R.T.: 0.042 min
Response: 288961
Conc: 2.11 ug/ml

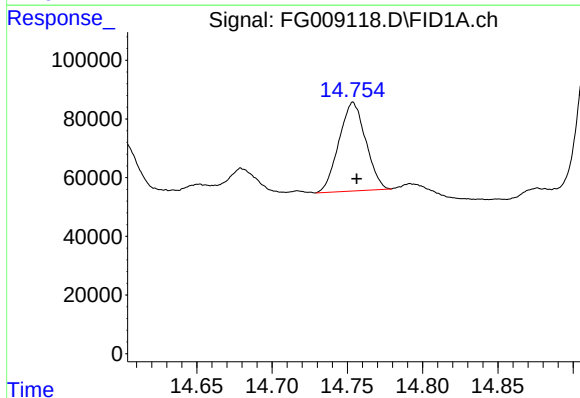


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.754 min
Delta R.T.: -0.002 min
Response: 374181
Conc: 3.21 ug/ml

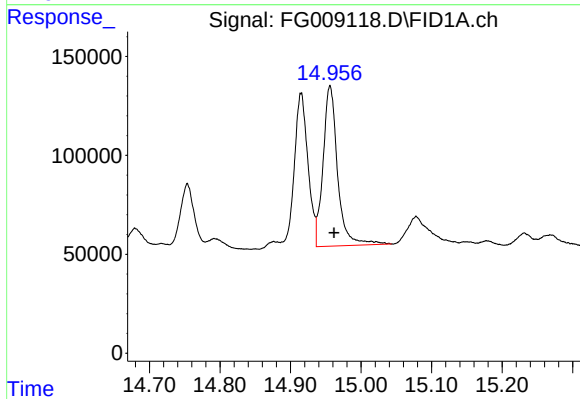

#10 N-TETRACOSANE


R.T.: 14.956 min
Delta R.T.: -0.006 min
Response: 1160673
Conc: 8.82 ug/ml

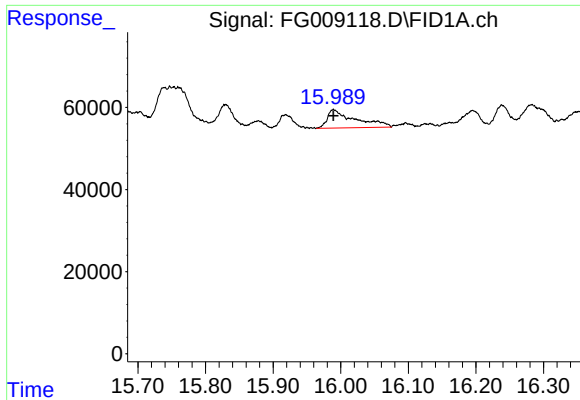

#11 N-HEXACOSANE


R.T.: 15.989 min
Delta R.T.: 0.000 min
Response: 127432
Conc: 1.04 ug/ml

Instrument :
FID_G
ClientSampleId :

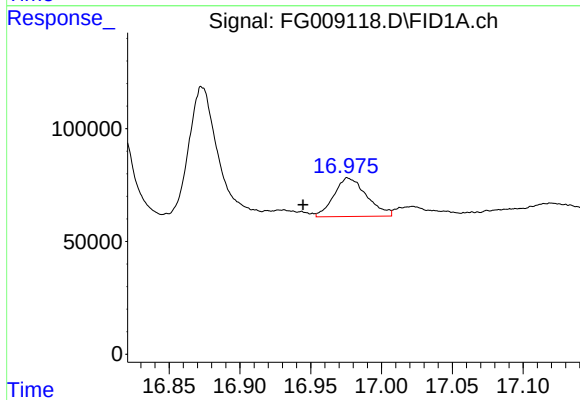


#12 N-OCTACOSANE

R.T.: 16.976 min
Delta R.T.: 0.032 min
Response: 276023
Conc: 2.42 ug/ml

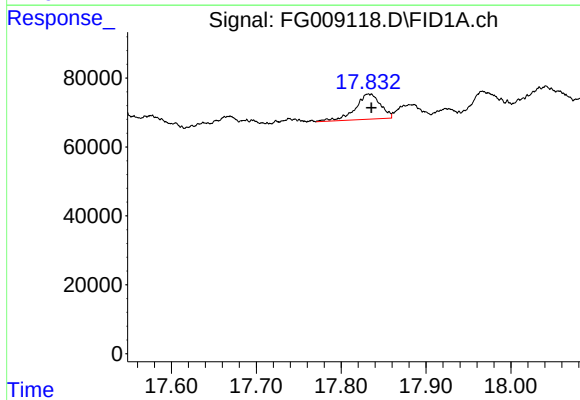


#13 N-TRIACONTANE

R.T.: 17.833 min
Delta R.T.: -0.003 min
Response: 149790
Conc: 1.38 ug/ml

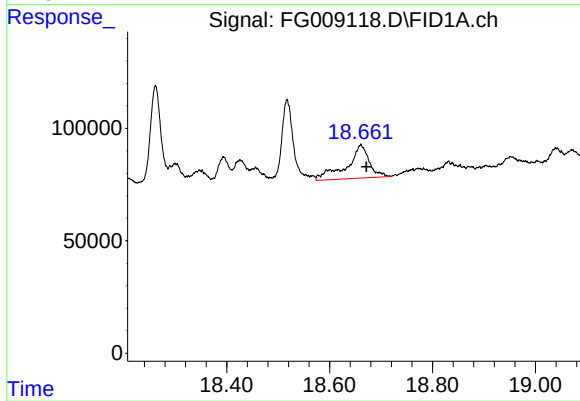

#14 N-DOTRIACONTANE


R.T.: 18.661 min
Delta R.T.: -0.011 min
Response: 447683
Conc: 4.35 ug/ml

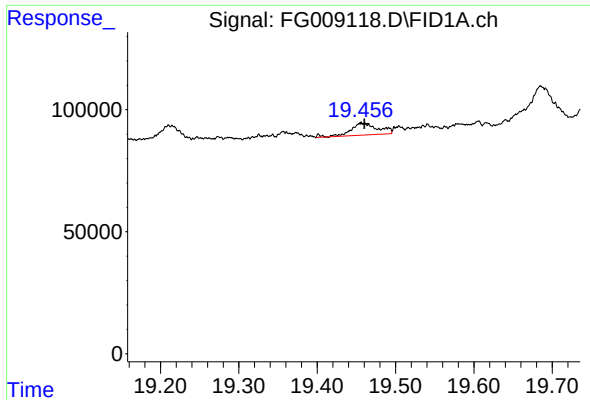

#15 N-TETRATRIACONTANE

R.T.: 19.457 min
Delta R.T.: -0.004 min
Response: 117725
Conc: 1.19 ug/ml

Instrument :
FID_G
ClientSampleId :

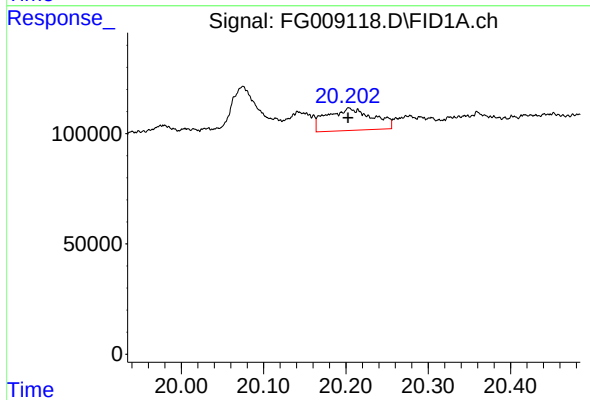

#16 N-HEXATRIACONTANE

R.T.: 20.204 min
Delta R.T.: 0.002 min
Response: 389919
Conc: 4.15 ug/ml