

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120221\
Data File : FG009127.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2021 10:00
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 02 23:59:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.679	37097	0.361 ug/ml
15)	N-TETRATRIACONTANE	19.465	154296	1.560 ug/ml
16)	N-HEXATRIACONTANE	20.211	22525	0.240 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120221\
Data File : FG009127.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2021 10:00
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 02 23:59:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

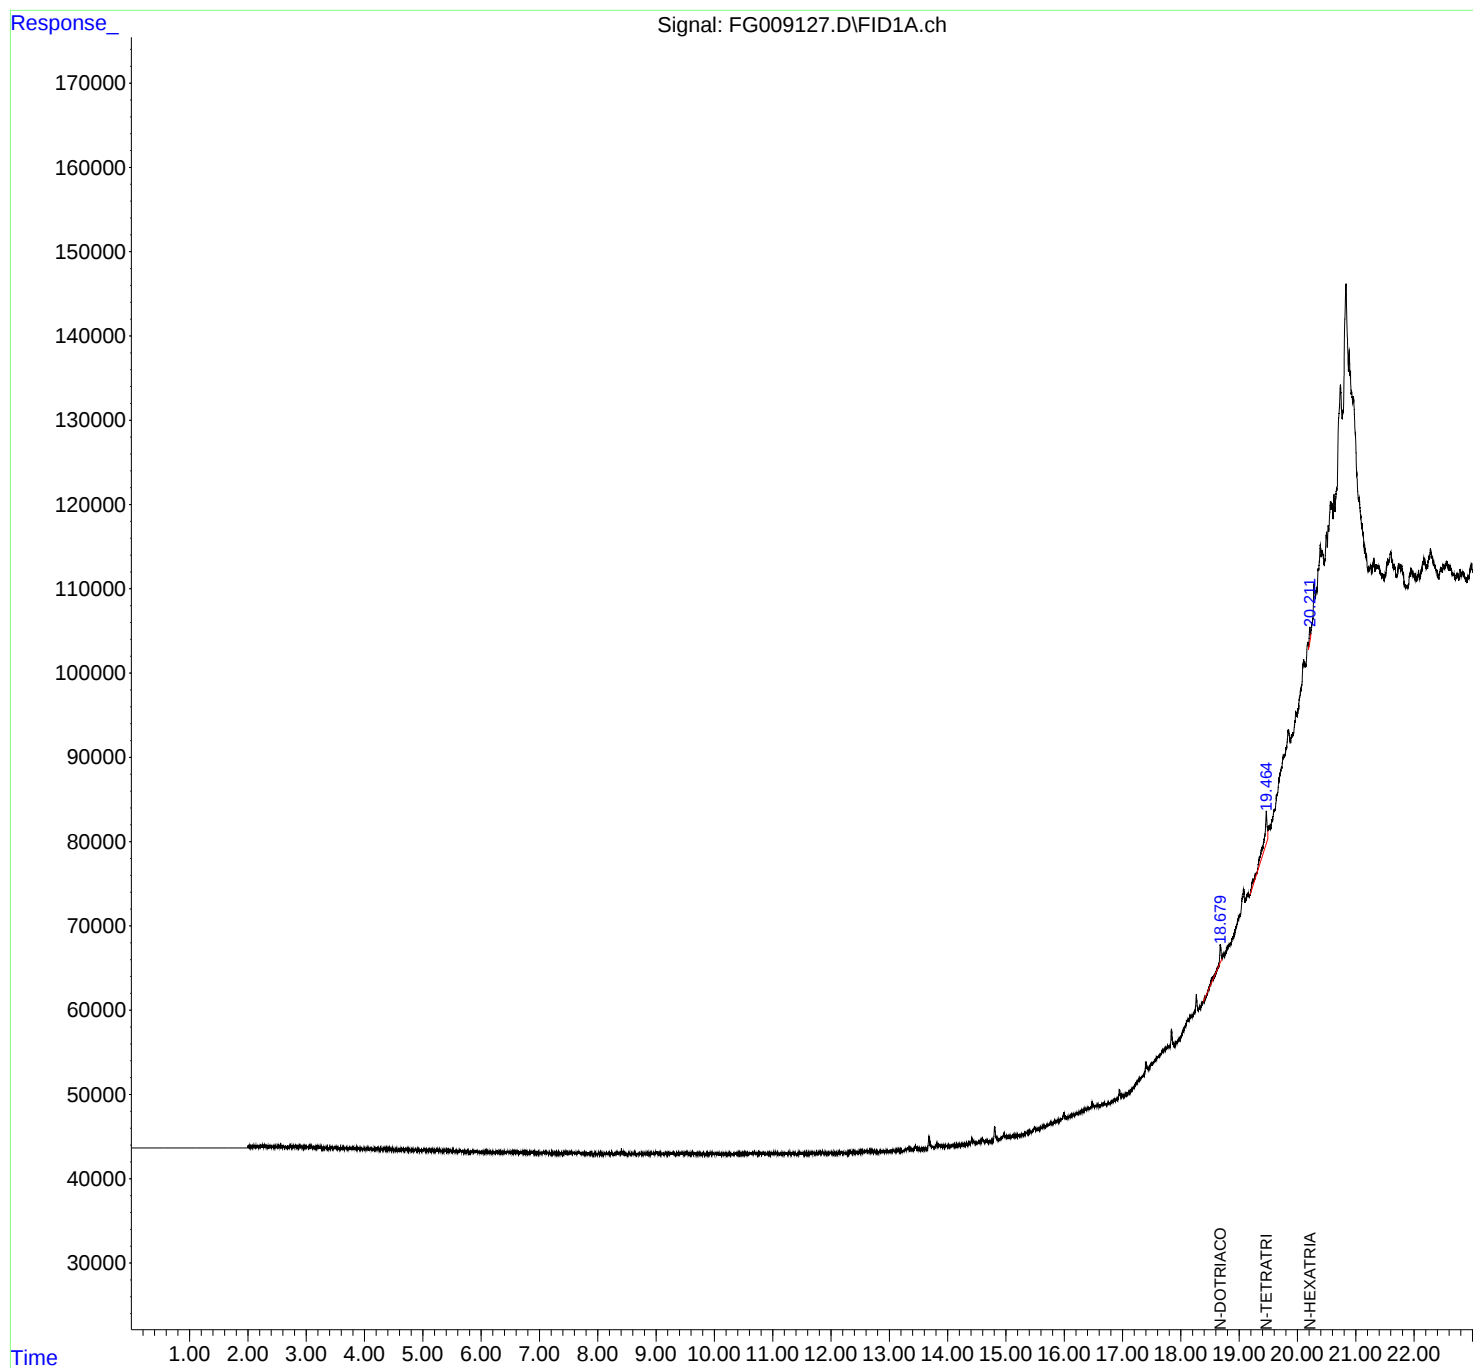


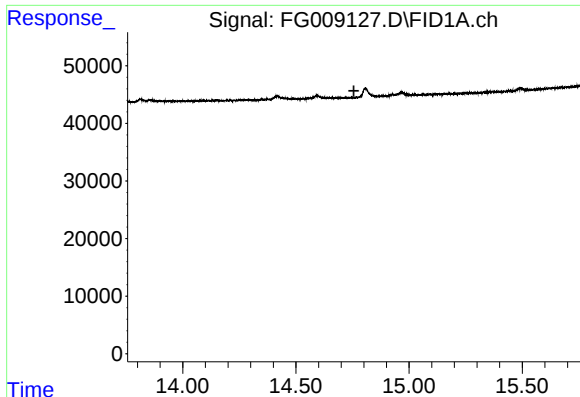

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.756 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

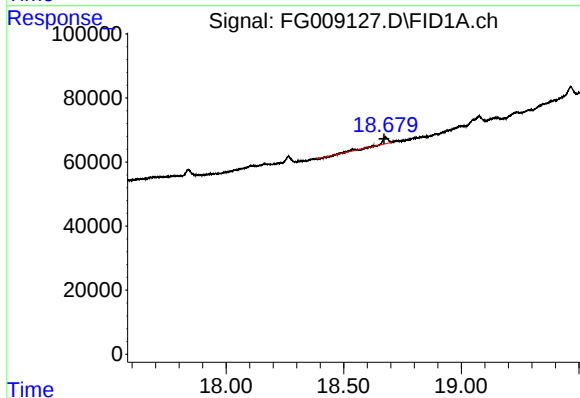


#14 N-DOTRIACONTANE

R.T.: 18.679 min
Delta R.T.: 0.008 min
Response: 37097
Conc: 0.36 ug/ml

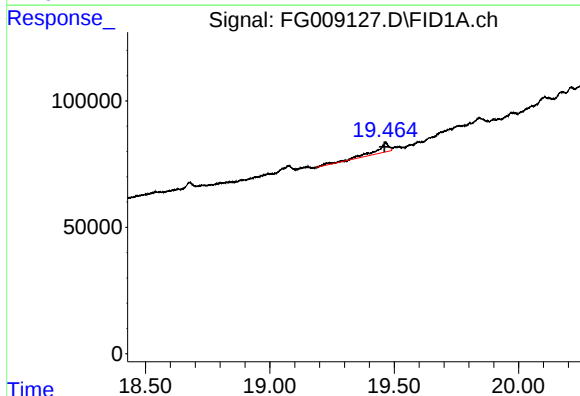

#15 N-TETRATRIACONTANE

R.T.: 19.465 min
Delta R.T.: 0.004 min
Response: 154296
Conc: 1.56 ug/ml

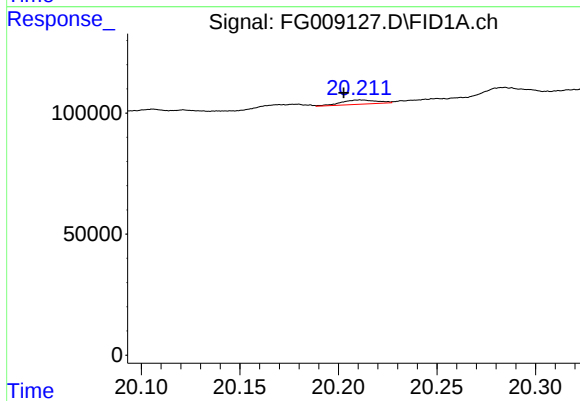

#16 N-HEXATRIACONTANE

R.T.: 20.211 min
Delta R.T.: 0.009 min
Response: 22525
Conc: 0.24 ug/ml