

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120221\
 Data File : FG009132.D
 Signal(s) : FID1A.ch
 Acq On : 02 Dec 2021 12:50
 Operator : AJ\MA
 Sample : M4893-03DL 25X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 03 00:01:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
 Quant Title :
 QLast Update : Wed Nov 24 00:59:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.760	54256	0.465 ug/ml
Target Compounds			
7) N-EICOSANE	12.644	83152	0.581 ug/ml
8) N-DOCOSANE	13.901	154116	1.123 ug/ml
10) N-TETRACOSANE	14.965	468659	3.561 ug/ml
12) N-OCTACOSANE	16.987	47633	0.418 ug/ml
13) N-TRIACONTANE	17.840	62589	0.579 ug/ml
14) N-DOTRIACONTANE	18.674	110160	1.071 ug/ml
15) N-TETRATRIACONTANE	19.466	78388	0.793 ug/ml
16) N-HEXATRIACONTANE	20.209	209456	2.229 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120221\
Data File : FG009132.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2021 12:50
Operator : AJ\MA
Sample : M4893-03DL 25X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 03 00:01:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

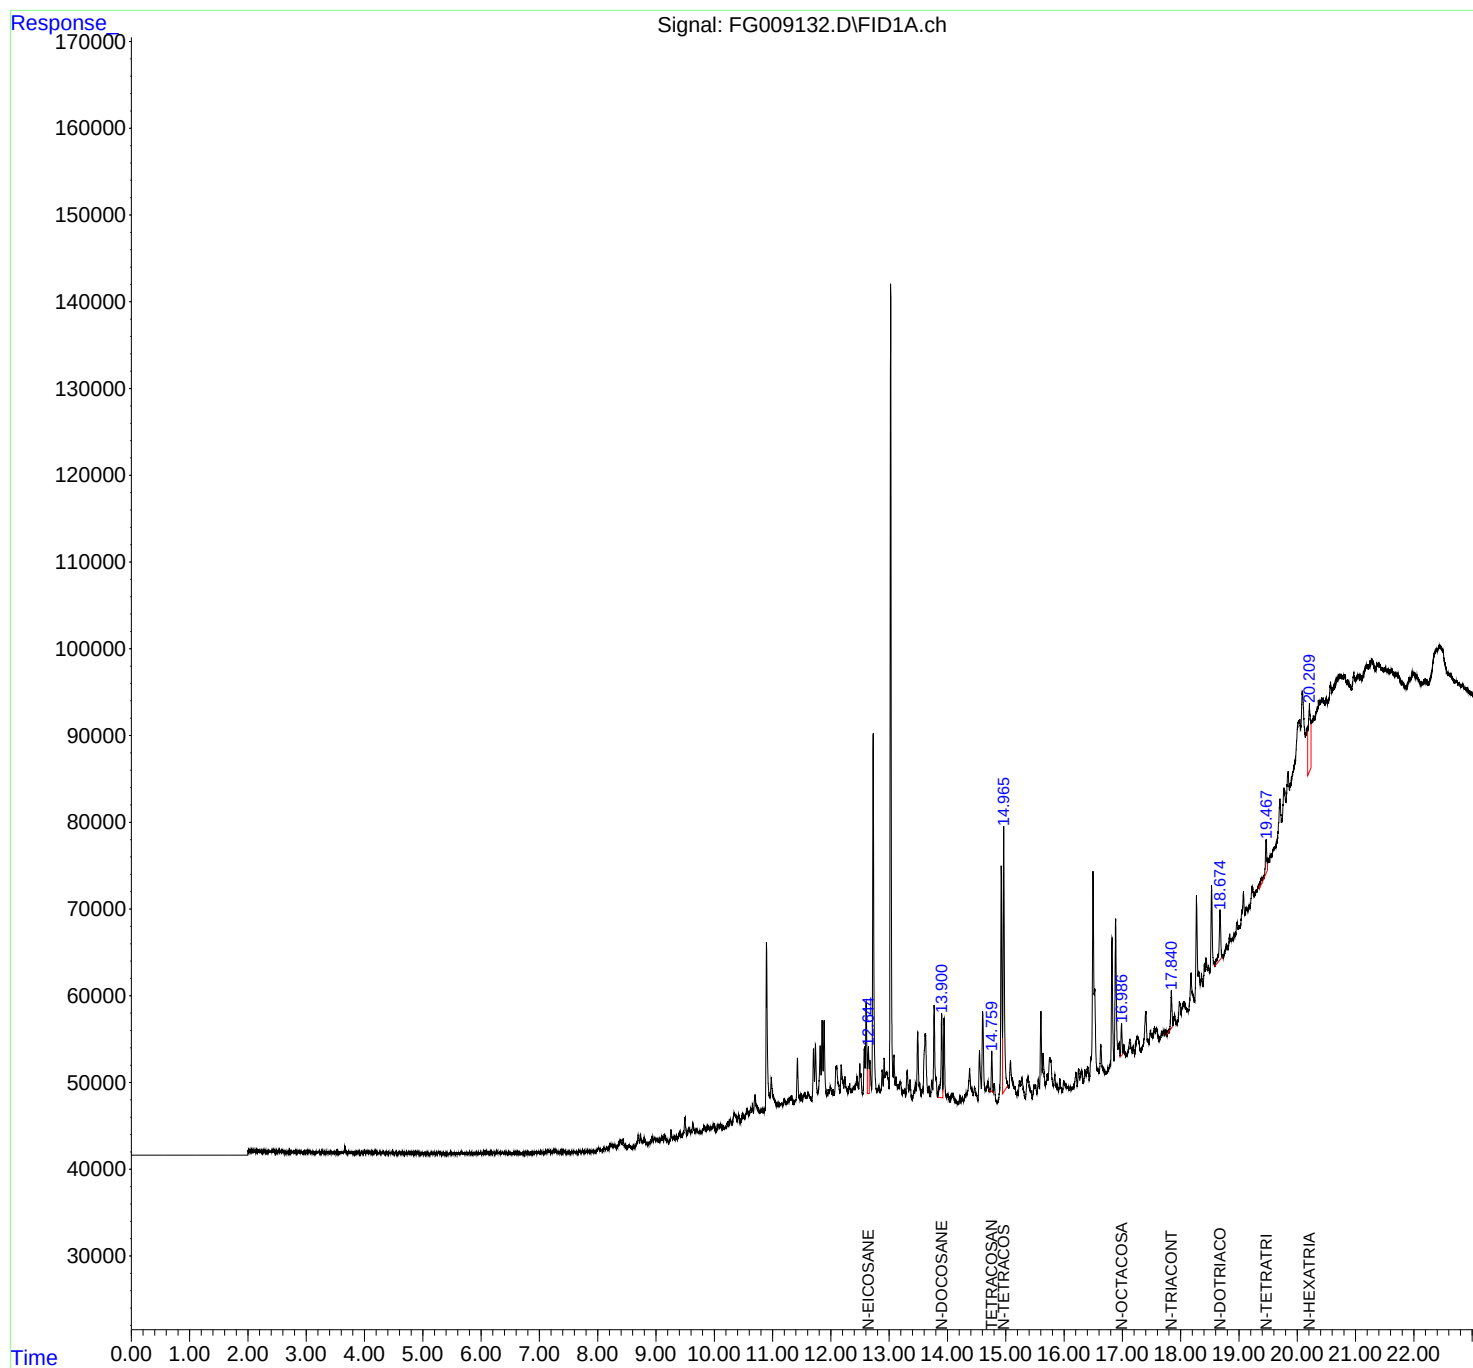


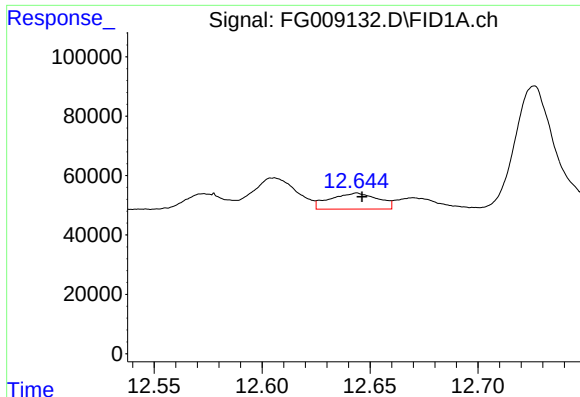

#7 N-EICOSANE


R.T.: 12.644 min
Delta R.T.: -0.002 min
Response: 83152
Conc: 0.58 ug/ml

Instrument :
FID_G
ClientSampleId :

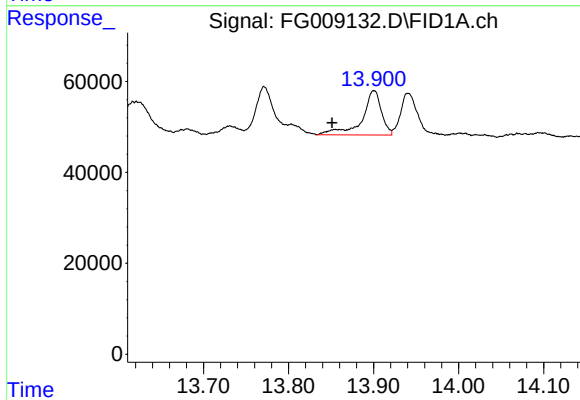


#8 N-DOCOSANE

R.T.: 13.901 min
Delta R.T.: 0.049 min
Response: 154116
Conc: 1.12 ug/ml

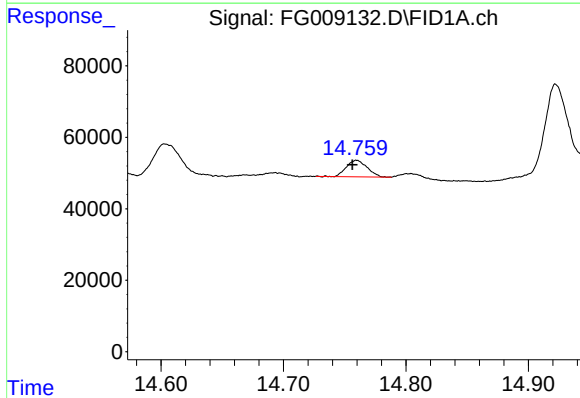


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.760 min
Delta R.T.: 0.004 min
Response: 54256
Conc: 0.47 ug/ml

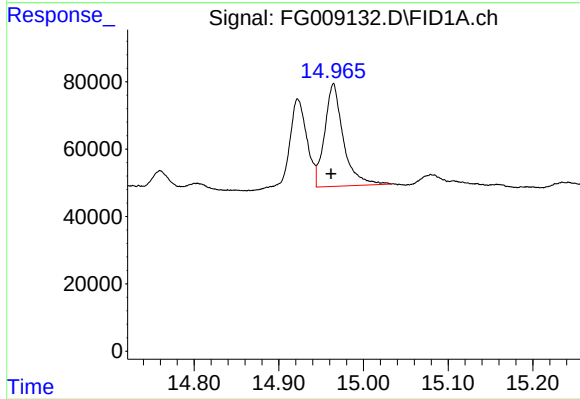

#10 N-TETRACOSANE


R.T.: 14.965 min
Delta R.T.: 0.003 min
Response: 468659
Conc: 3.56 ug/ml

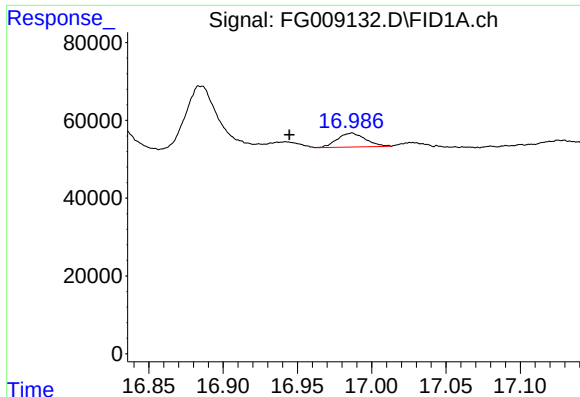

#12 N-OCTACOSANE


R.T.: 16.987 min
Delta R.T.: 0.042 min
Response: 47633
Conc: 0.42 ug/ml

Instrument :
FID_G
ClientSampleId :

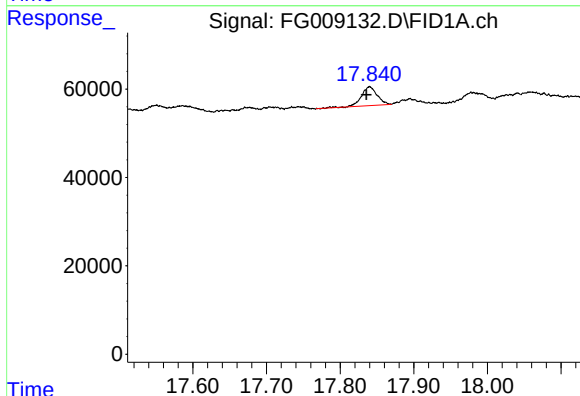


#13 N-TRIACONTANE

R.T.: 17.840 min
Delta R.T.: 0.004 min
Response: 62589
Conc: 0.58 ug/ml

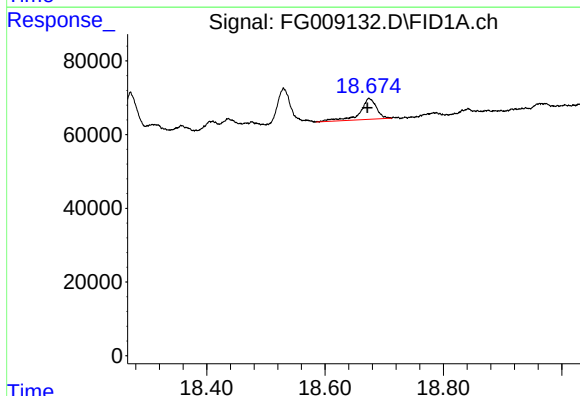


#14 N-DOTRIACONTANE

R.T.: 18.674 min
Delta R.T.: 0.003 min
Response: 110160
Conc: 1.07 ug/ml

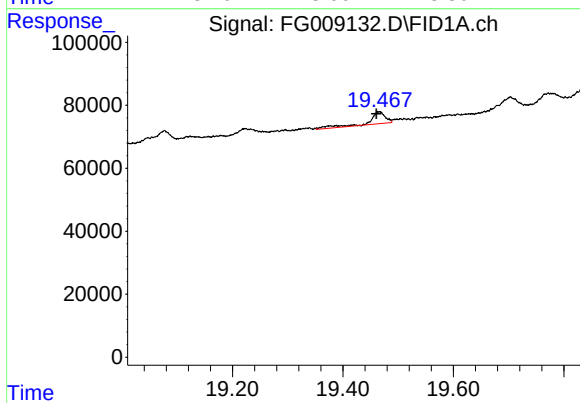

#15 N-TETRATRIACONTANE

R.T.: 19.466 min
Delta R.T.: 0.006 min
Response: 78388
Conc: 0.79 ug/ml

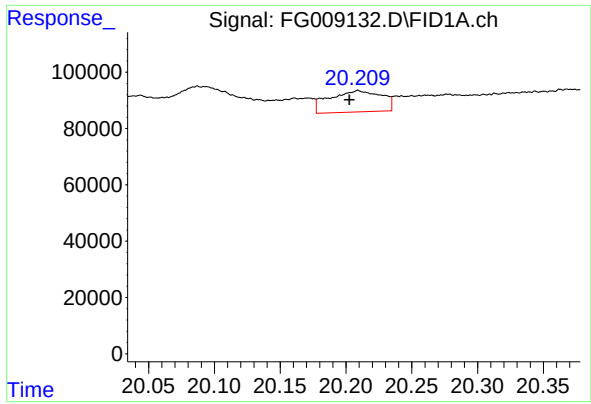

#16 N-HEXATRIACONTANE

R.T.: 20.209 min
Delta R.T.: 0.007 min
Response: 209456
Conc: 2.23 ug/ml

Instrument :
FID_G
ClientSampleId :