

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120221\
Data File : FG009130.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2021 11:33
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 03 00:00:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.468	2952675	19.947 ug/ml
12) N-OCTACOSANE	16.946	2496789	21.898 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120221\
Data File : FG009130.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2021 11:33
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 03 00:00:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

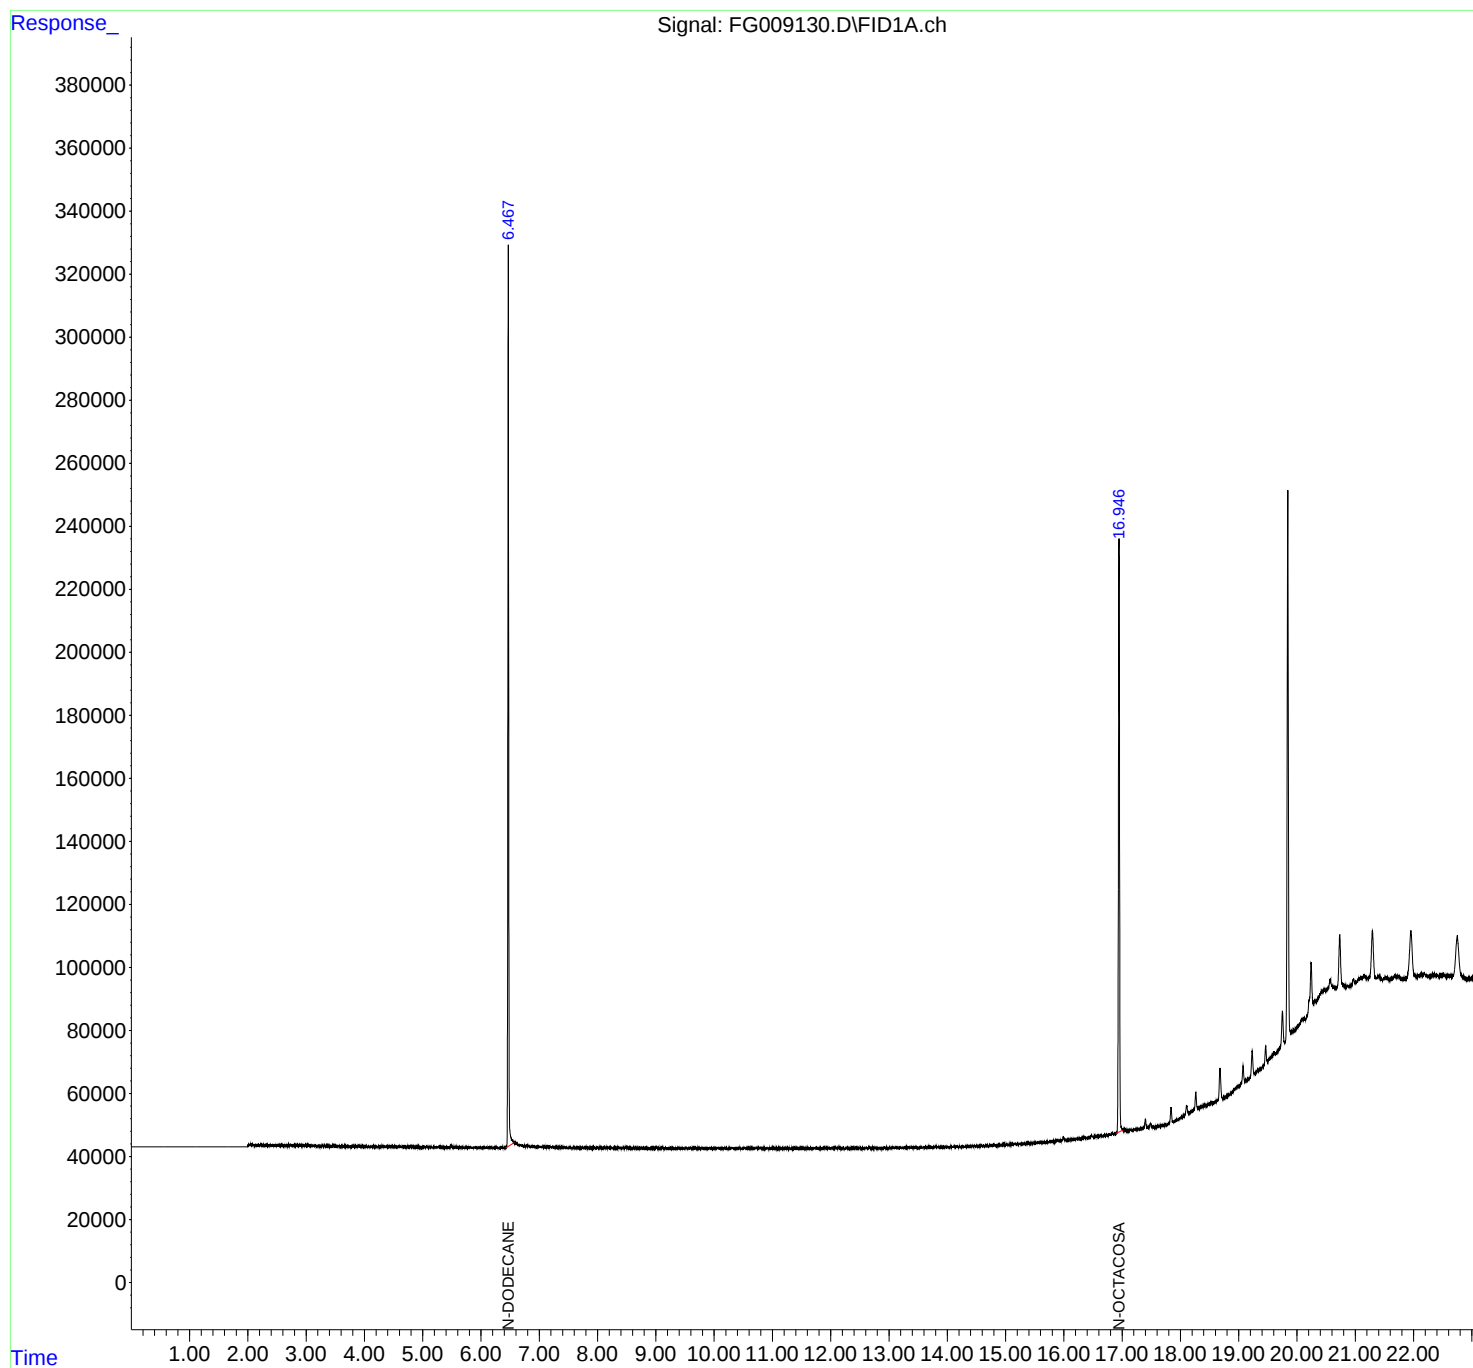


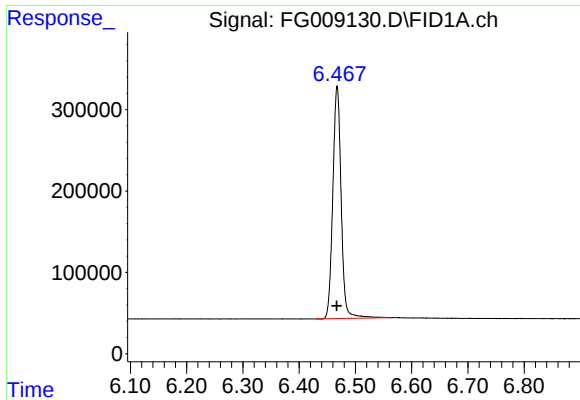

#3 N-DODECANE


R.T.: 6.468 min
Delta R.T.: 0.000 min
Response: 2952675
Conc: 19.95 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

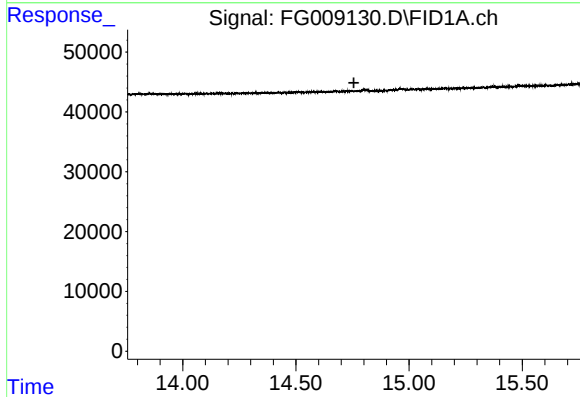

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.756 min
Response: 0
Conc: N.D.

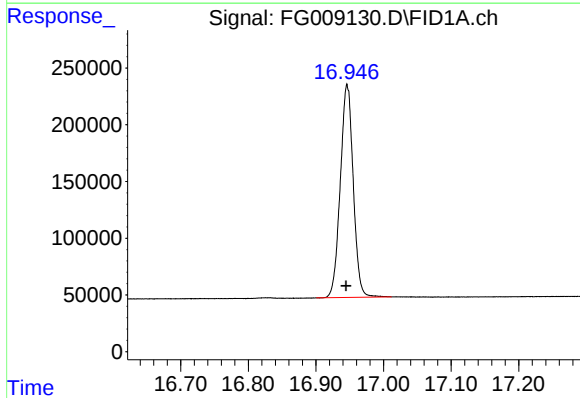

#12 N-OCTACOSANE

R.T.: 16.946 min
Delta R.T.: 0.001 min
Response: 2496789
Conc: 21.90 ug/ml