

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120222\
Data File : FG011170.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2022 10:54
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 04 10:59:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
Quant Title :
QLast Update : Mon Nov 14 17:25:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) N-TETRACOSANE	15.259	2926847	23.363 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120222\
Data File : FG011170.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2022 10:54
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 04 10:59:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
Quant Title :
QLast Update : Mon Nov 14 17:25:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

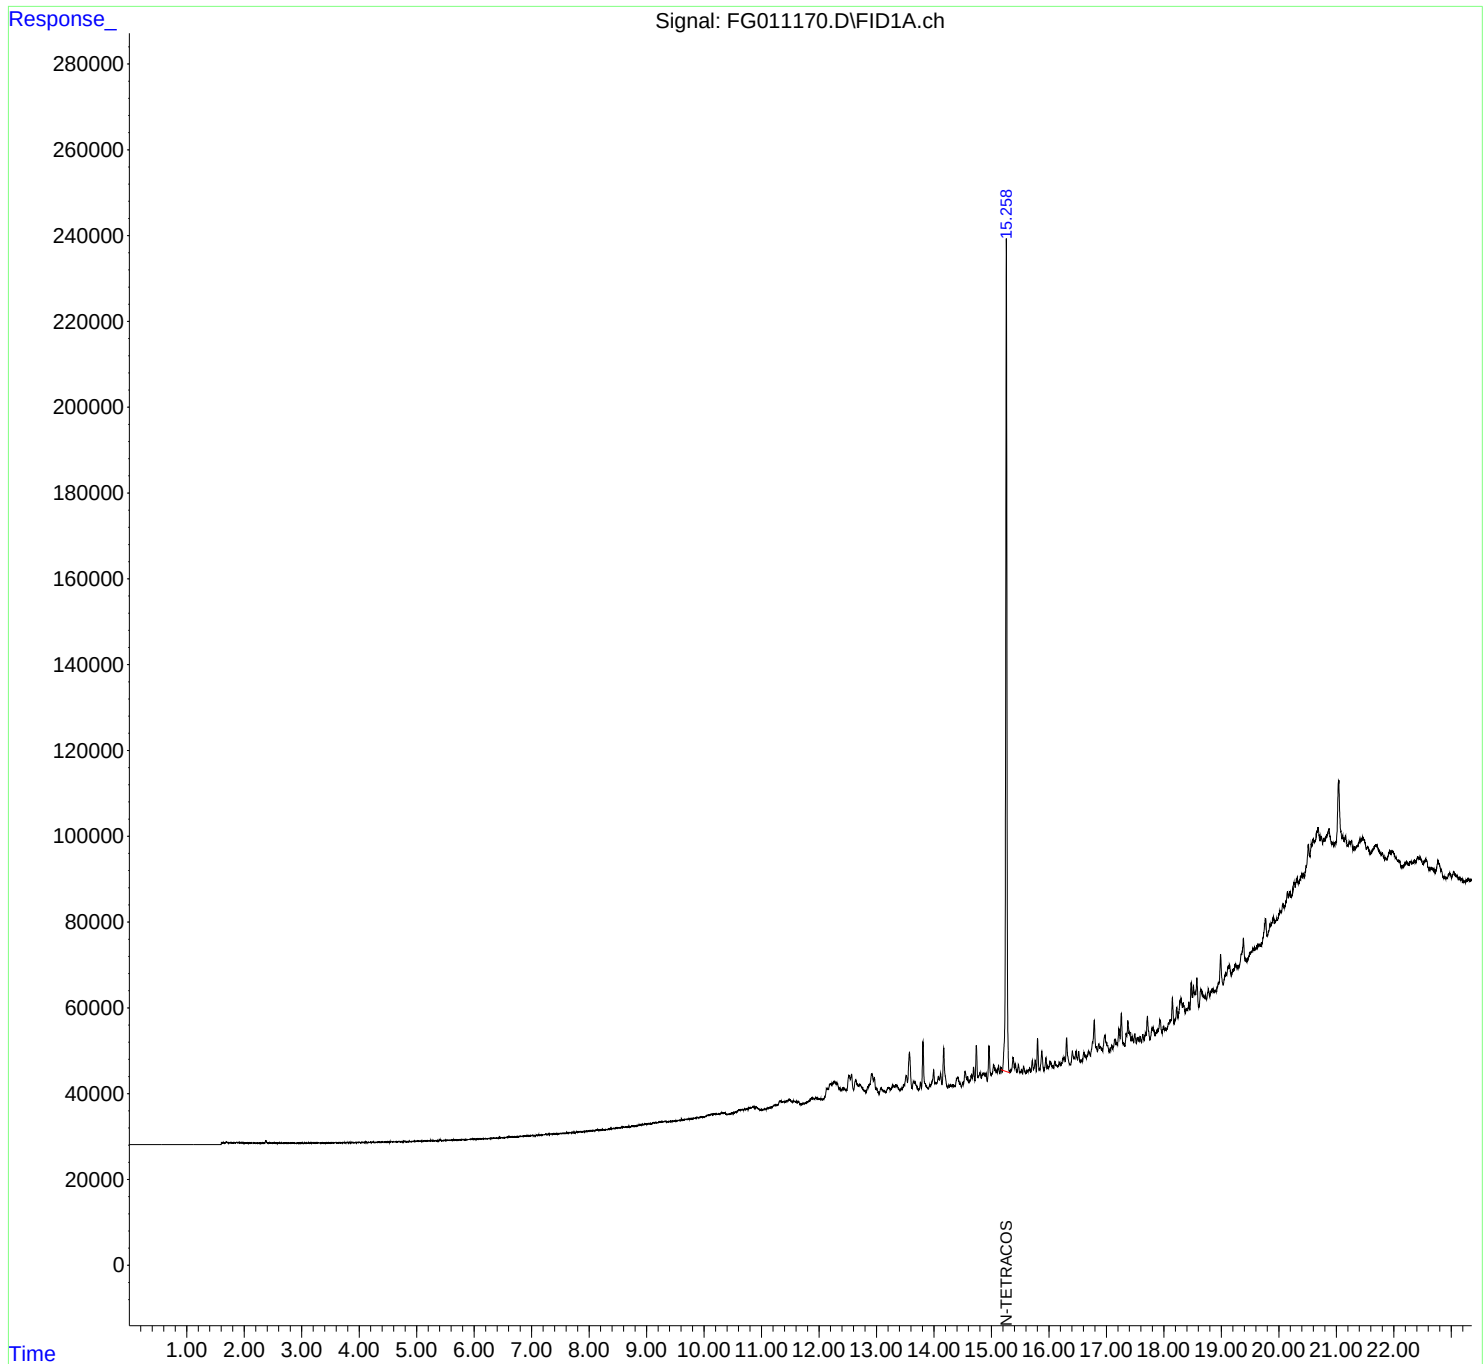


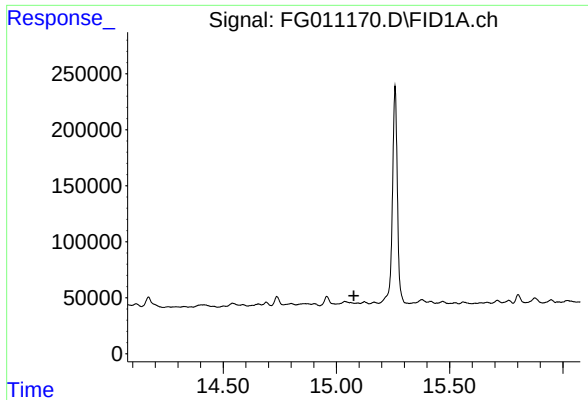

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.077 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

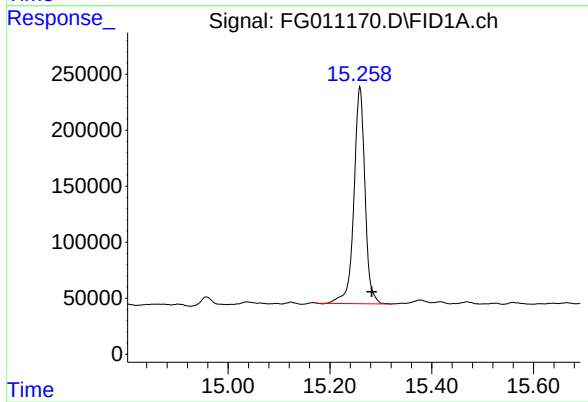

#10 N-TETRACOSANE

R.T.: 15.259 min
Delta R.T.: -0.023 min
Response: 2926847
Conc: 23.36 ug/ml