

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120222\
Data File : FG011176.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2022 15:00
Operator : YP\AJ
Sample : N5846-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SP25-10-20221201-6.5-7.0

Integration File: Sample.e
Quant Time: Dec 04 11:01:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
Quant Title :
QLast Update : Mon Nov 14 17:25:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.080	3219750	29.411 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120222\
Data File : FG011176.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2022 15:00
Operator : YP\AJ
Sample : N5846-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SP25-10-20221201-6.5-7.0

Integration File: Sample.e
Quant Time: Dec 04 11:01:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
Quant Title :
QLast Update : Mon Nov 14 17:25:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

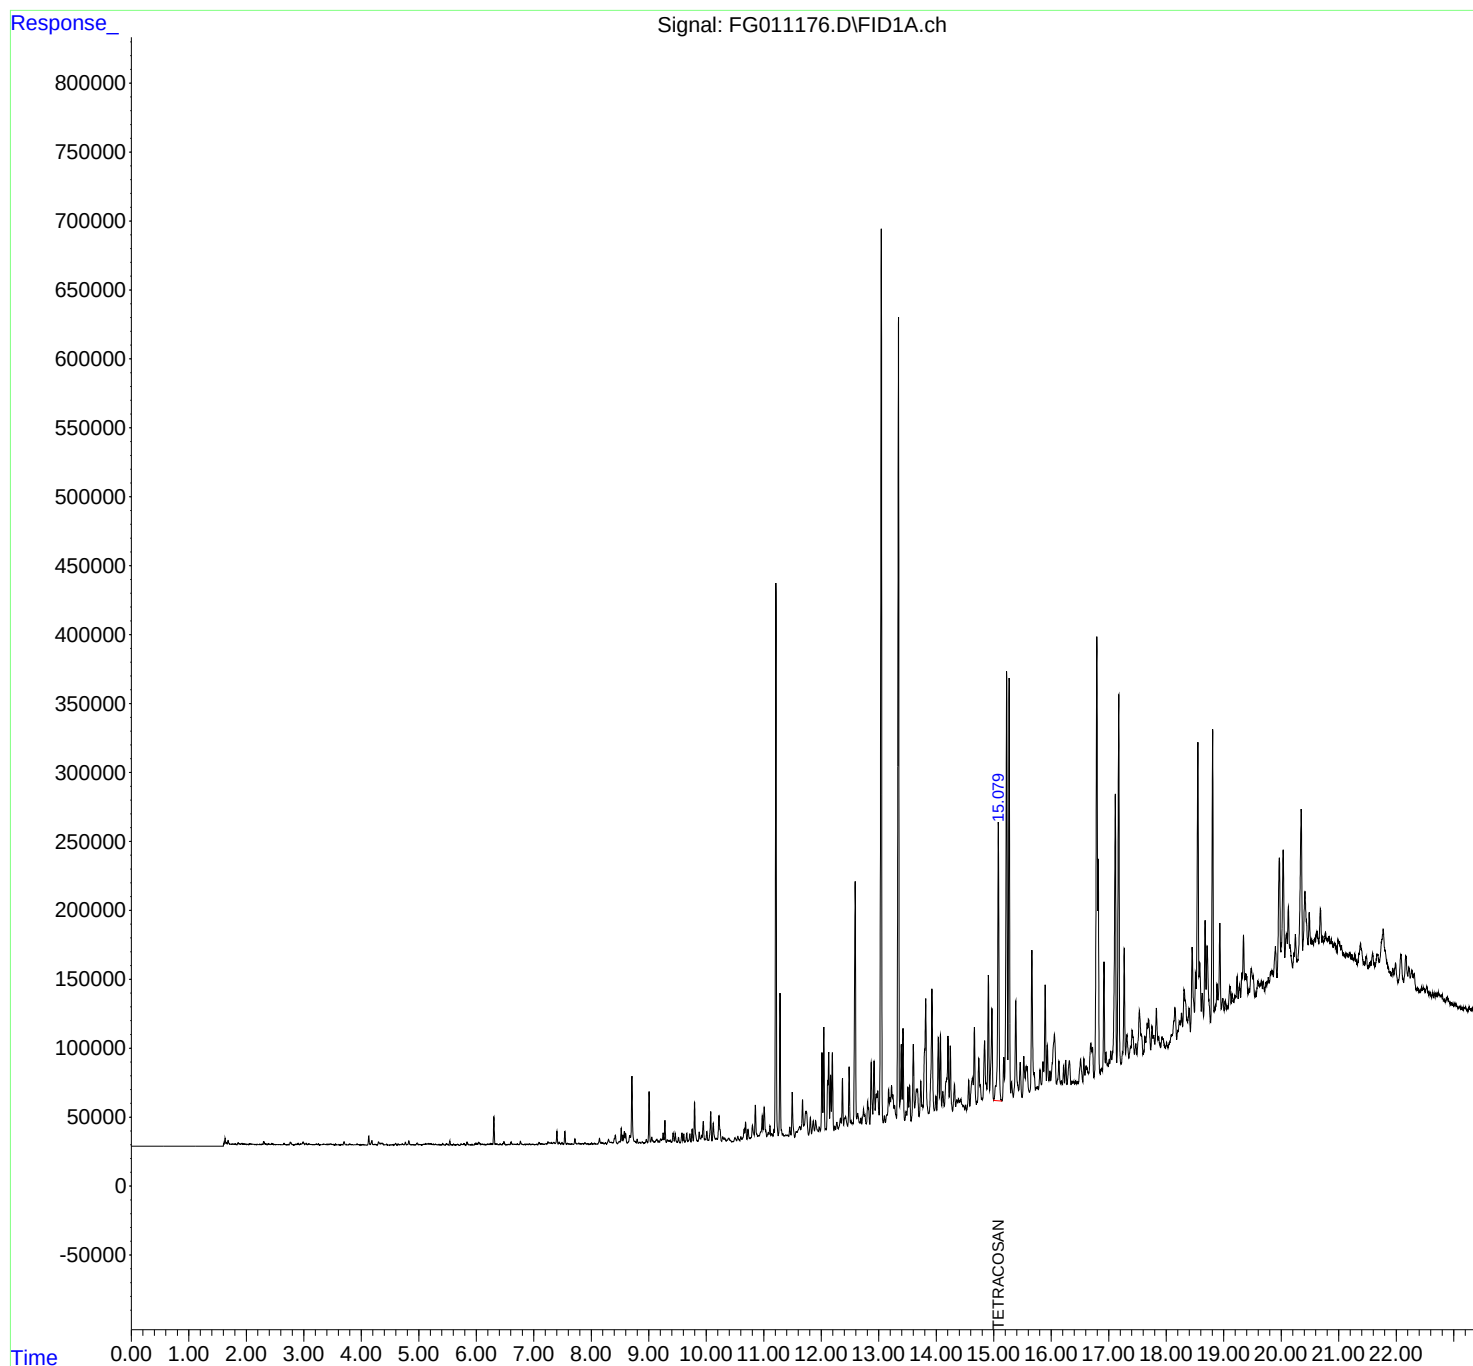

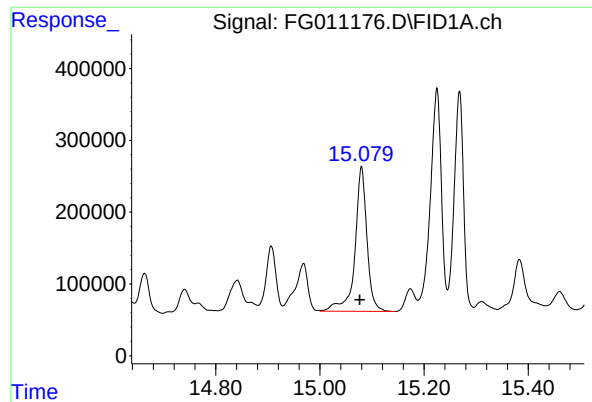

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.080 min
Delta R.T.: 0.003 min
Response: 3219750
Conc: 29.41 ug/ml

Instrument :

FID_G

ClientSampleId :

SP25-10-20221201-6.5-7.0