

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120222\
 Data File : FG011179.D
 Signal(s) : FID1A.ch
 Acq On : 02 Dec 2022 16:30
 Operator : YP\AJ
 Sample : N5846-04 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SP25-10-20221201-6.5-7.0

Integration File: Sample.e
 Quant Time: Dec 04 11:01:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
 Quant Title :
 QLast Update : Mon Nov 14 17:25:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.078	478474	4.371 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120222\
Data File : FG011179.D
Signal(s) : FID1A.ch
Acq On : 02 Dec 2022 16:30
Operator : YP\AJ
Sample : N5846-04 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SP25-10-20221201-6.5-7.0

Integration File: Sample.e
Quant Time: Dec 04 11:01:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG111422.M
Quant Title :
QLast Update : Mon Nov 14 17:25:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

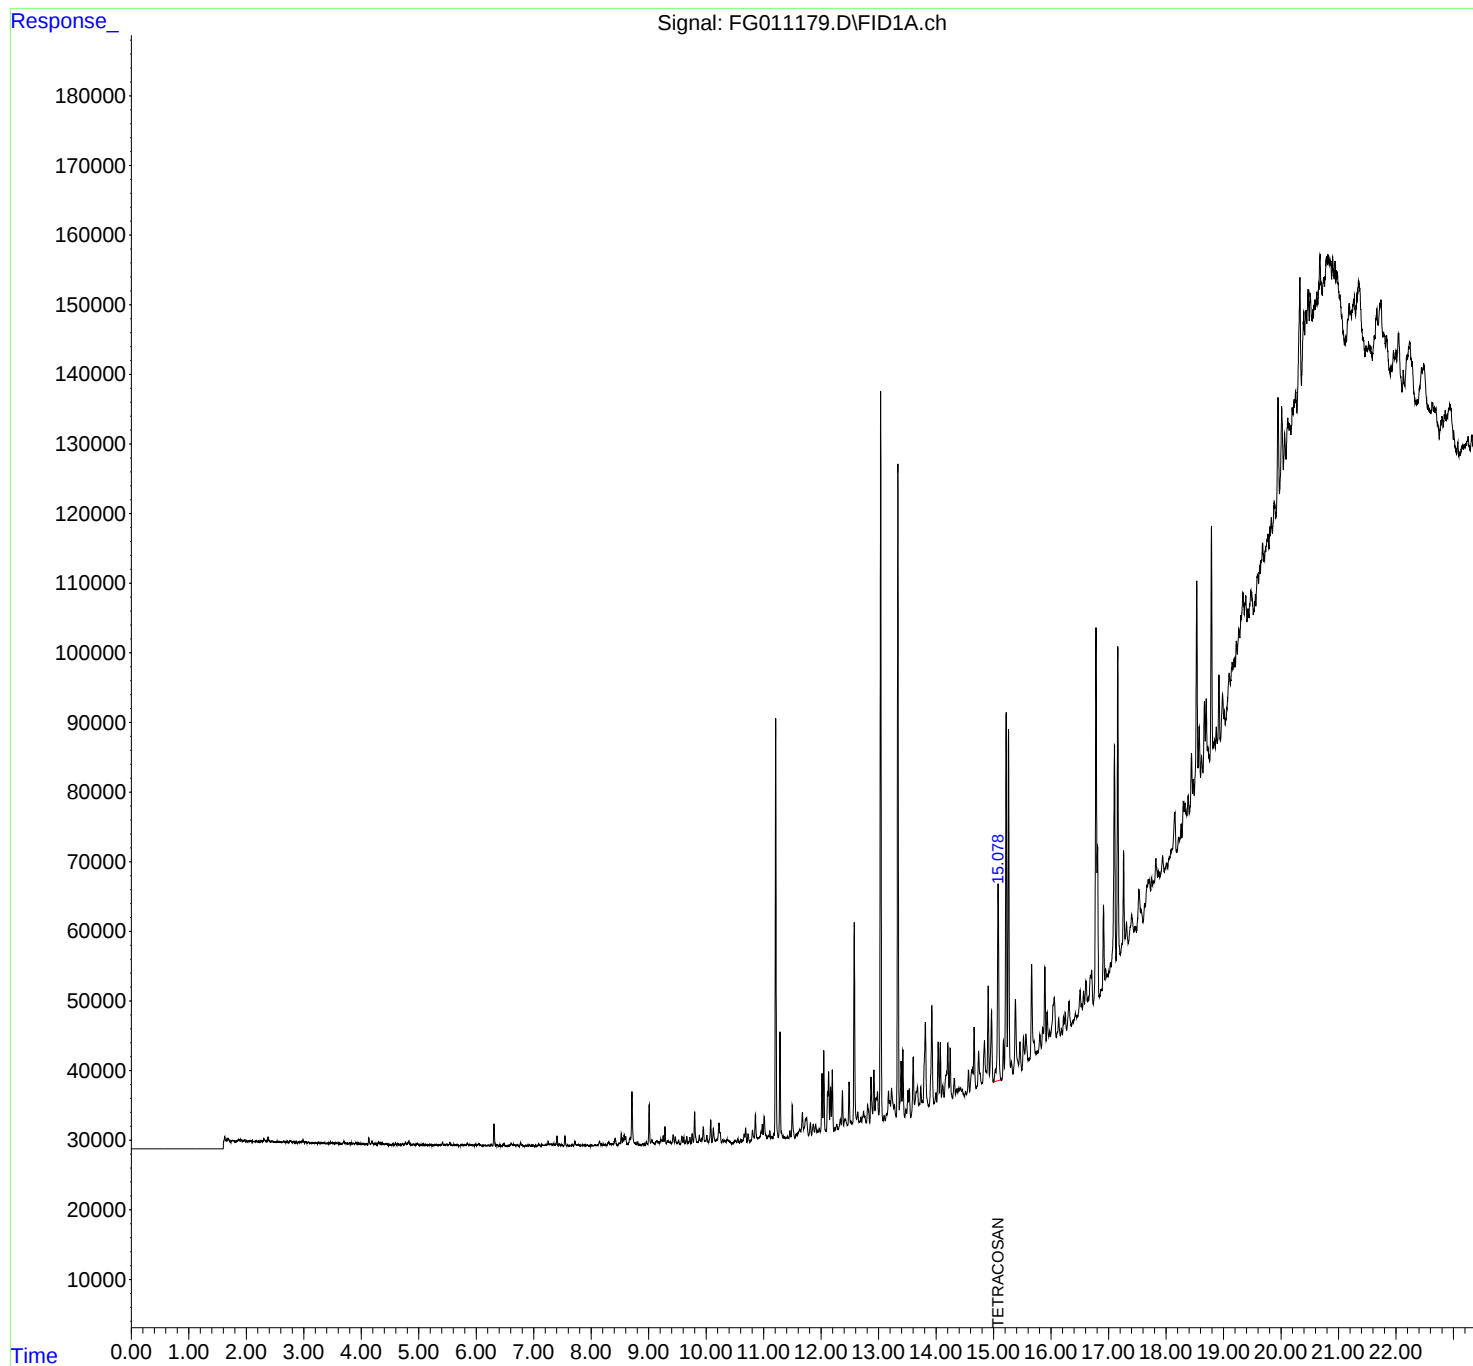

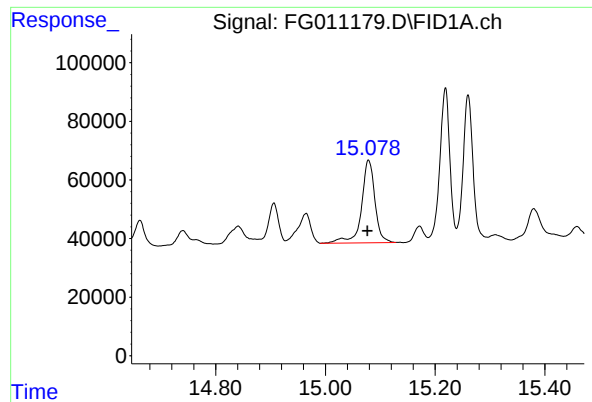

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.078 min
Delta R.T.: 0.001 min
Response: 478474
Conc: 4.37 ug/ml

Instrument :
FID_G
ClientSampleId :
SP25-10-20221201-6.5-7.0