

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120321\
Data File : FG009136.D
Signal(s) : FID1A.ch
Acq On : 03 Dec 2021 09:20
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 03 22:19:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.675	45469	0.442 ug/ml
15)	N-TETRATRIACONTANE	19.463	31890	0.322 ug/ml
16)	N-HEXATRIACONTANE	20.244	49545	0.527 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120321\
Data File : FG009136.D
Signal(s) : FID1A.ch
Acq On : 03 Dec 2021 09:20
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 03 22:19:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

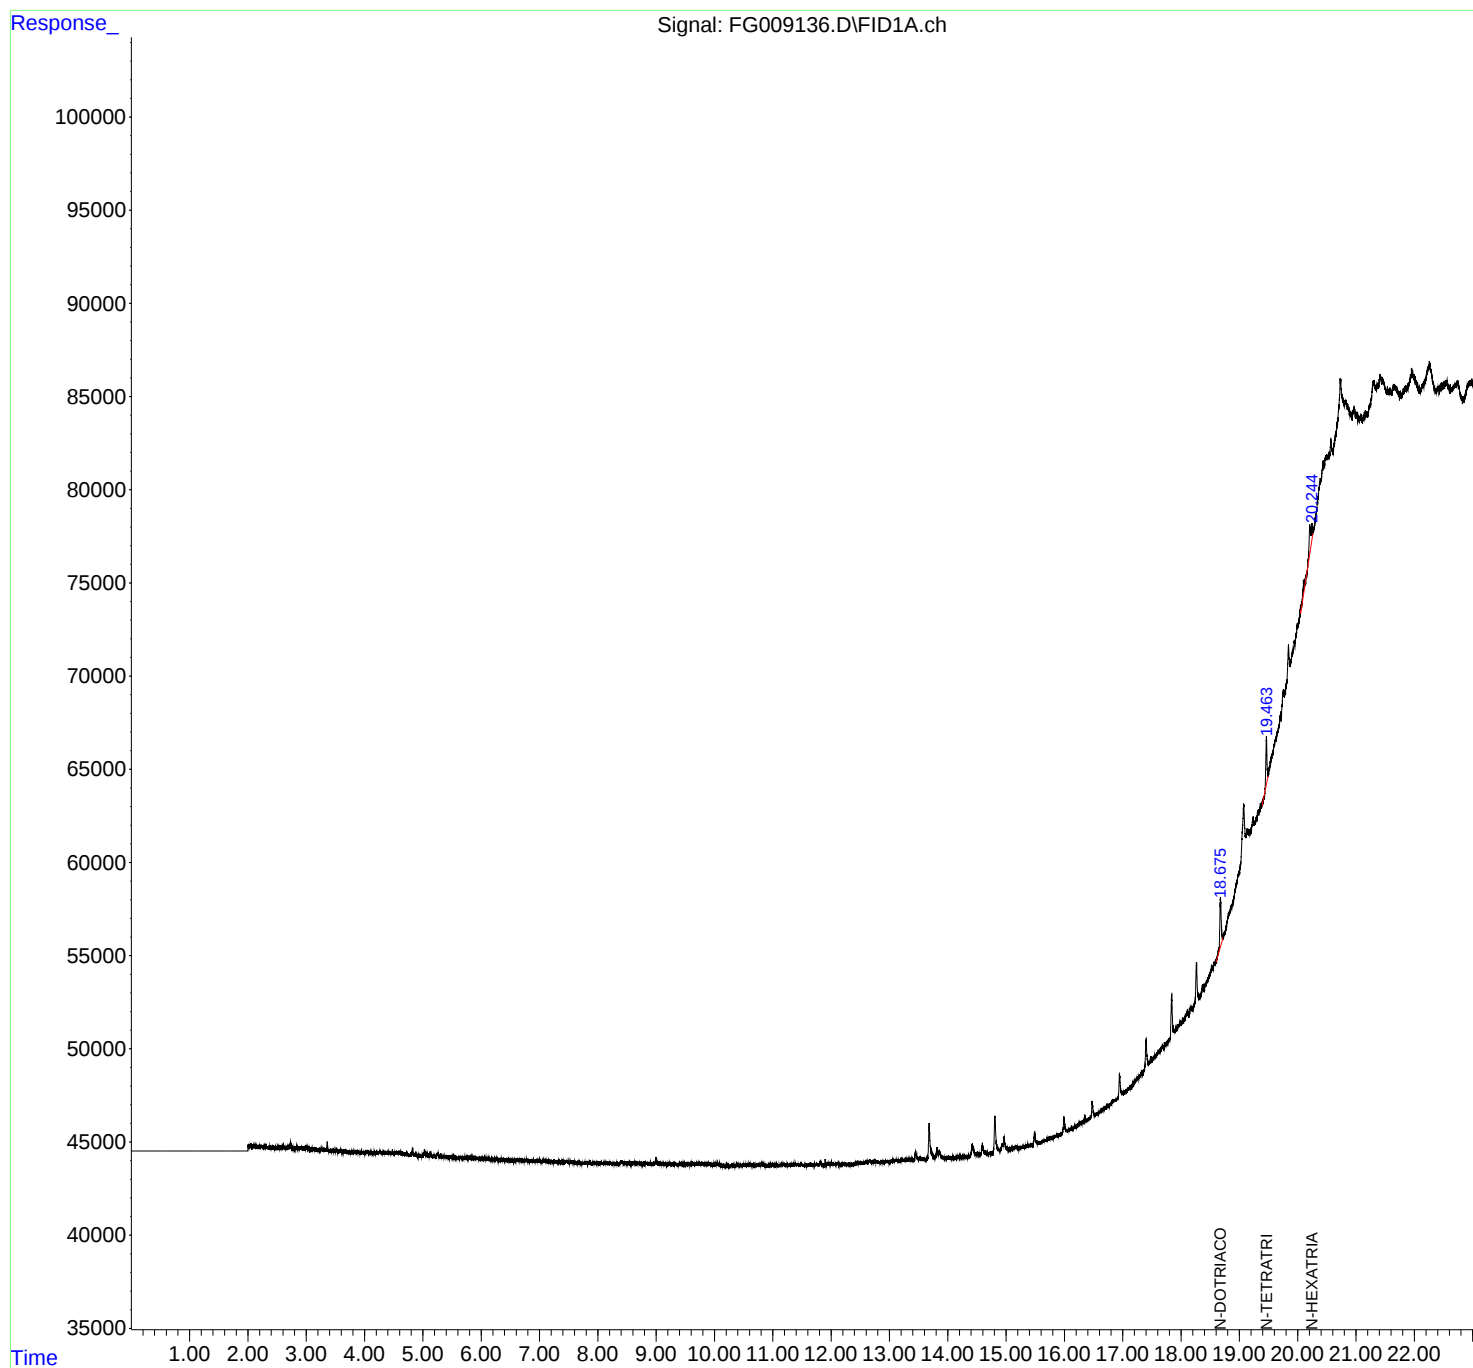


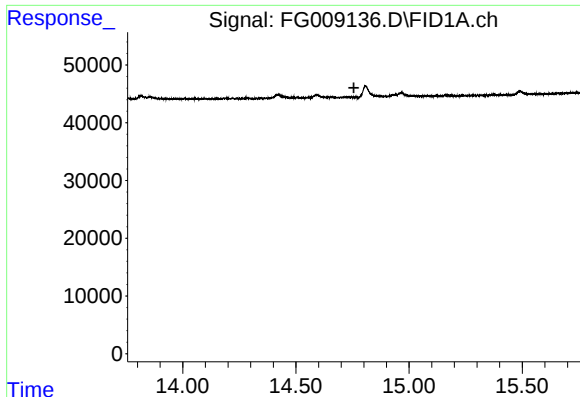

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.756 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

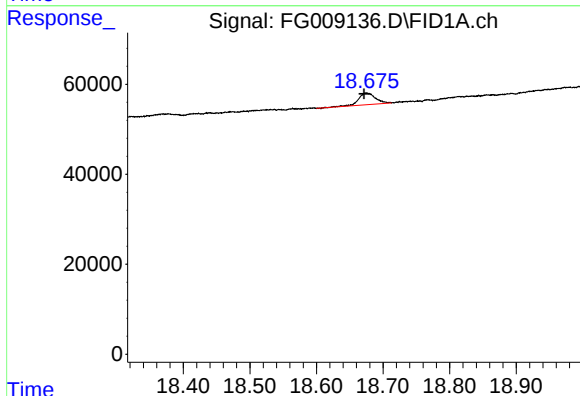


#14 N-DOTRIACONTANE

R.T.: 18.675 min
Delta R.T.: 0.004 min
Response: 45469
Conc: 0.44 ug/ml

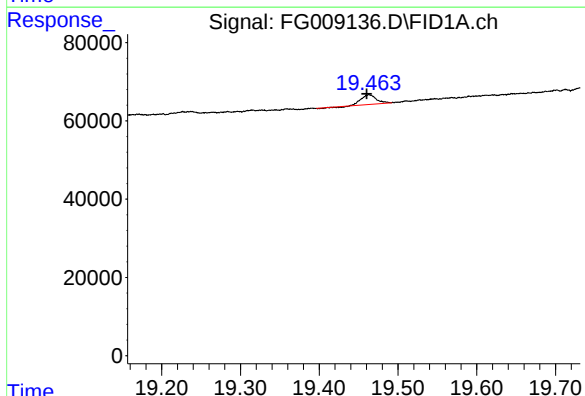

#15 N-TETRATRIACONTANE

R.T.: 19.463 min
Delta R.T.: 0.003 min
Response: 31890
Conc: 0.32 ug/ml

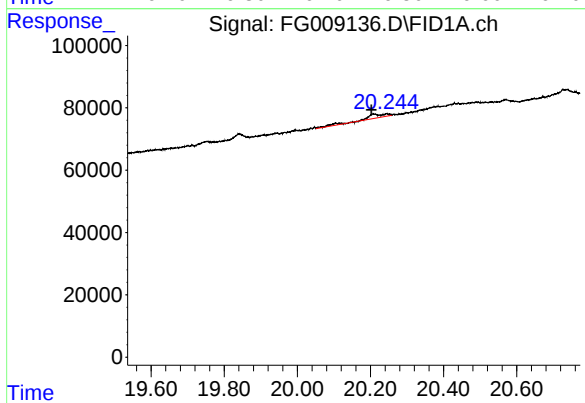

#16 N-HEXATRIACONTANE

R.T.: 20.244 min
Delta R.T.: 0.042 min
Response: 49545
Conc: 0.53 ug/ml