

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120321\
Data File : FG009156.D
Signal(s) : FID1A.ch
Acq On : 03 Dec 2021 23:10
Operator : AJ\MA
Sample : M4919-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 04 01:26:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.753	2173954	18.641 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.671	65164	0.634 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120321\
Data File : FG009156.D
Signal(s) : FID1A.ch
Acq On : 03 Dec 2021 23:10
Operator : AJ\MA
Sample : M4919-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 04 01:26:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

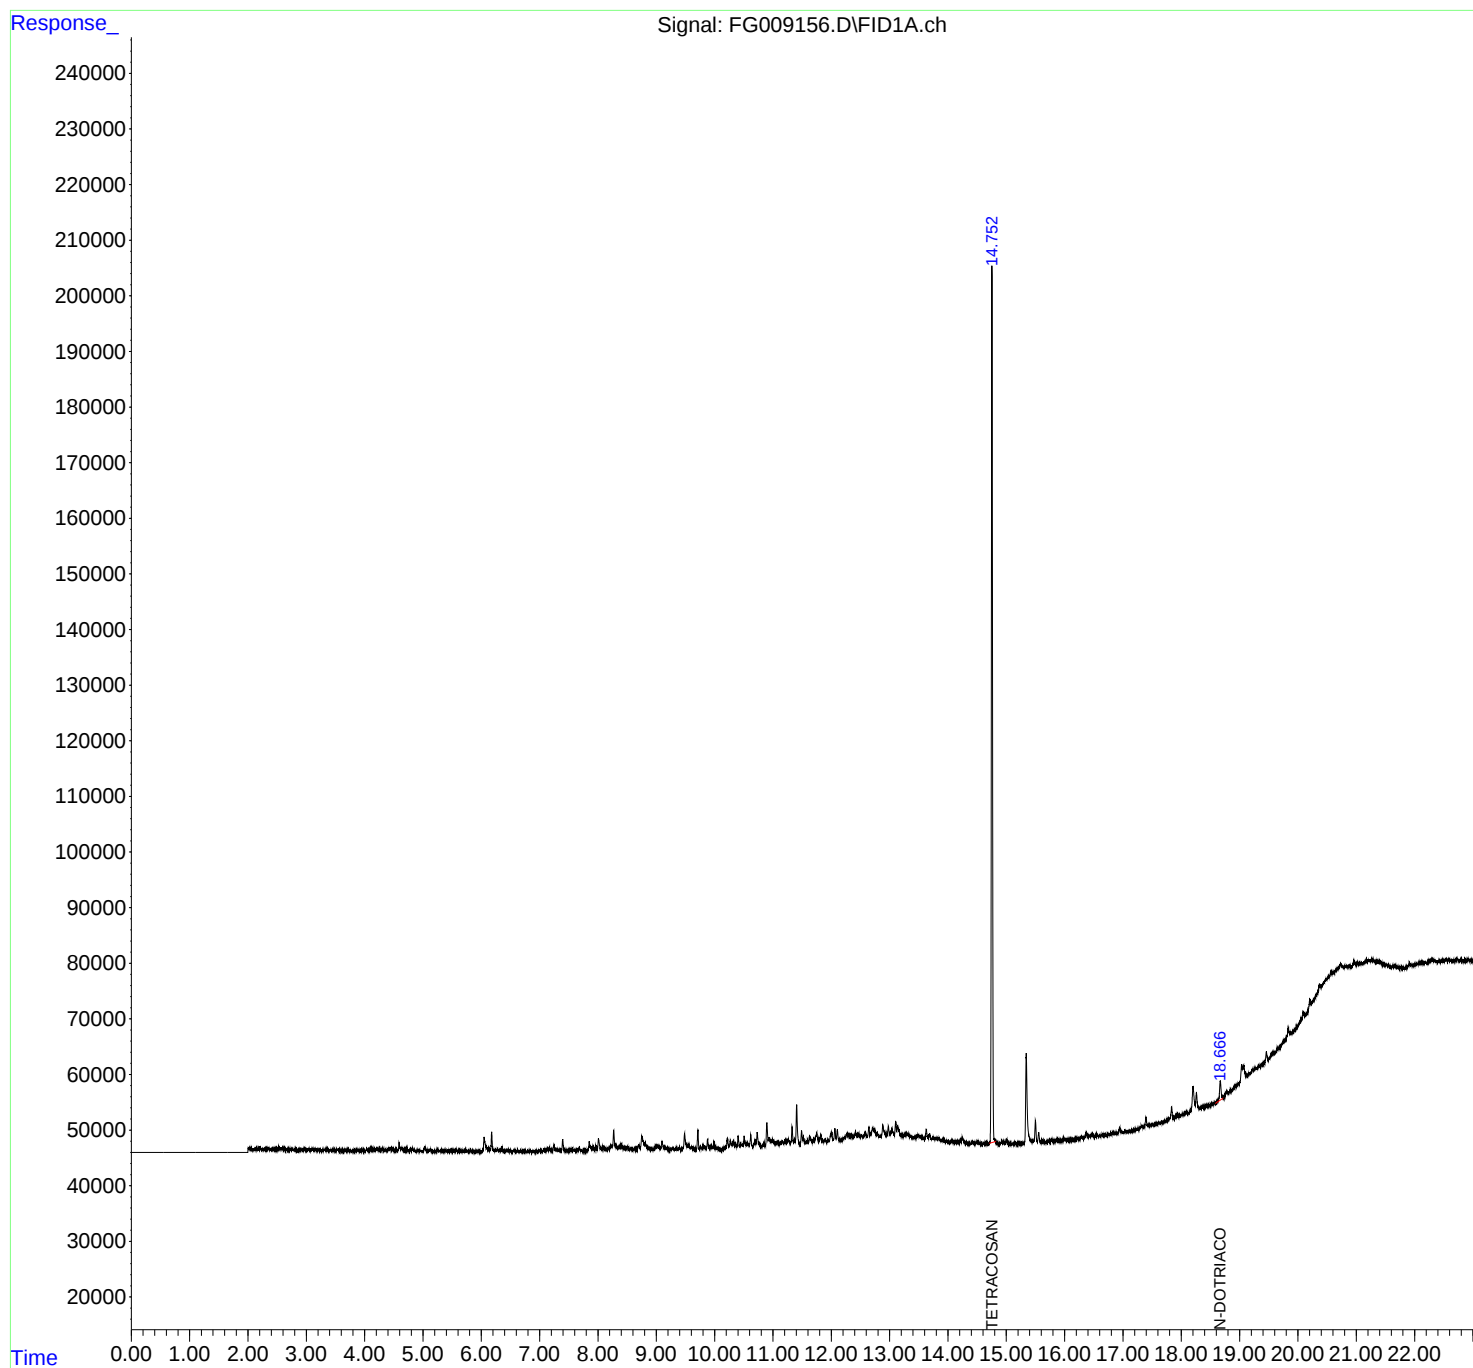


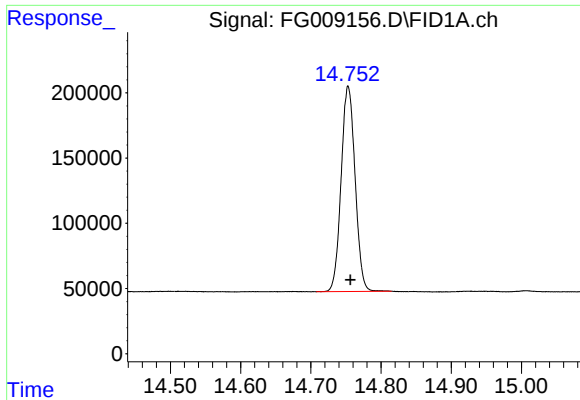

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.753 min
Delta R.T.: -0.003 min
Response: 2173954
Conc: 18.64 ug/ml

Instrument :
FID_G
ClientSampleId :

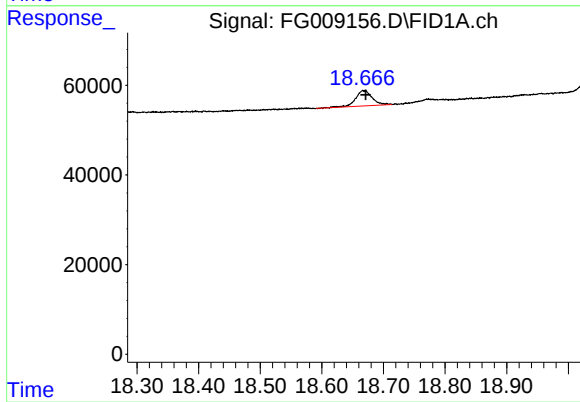

#14 N-DOTRIACONTANE

R.T.: 18.671 min
Delta R.T.: 0.000 min
Response: 65164
Conc: 0.63 ug/ml