

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120420\
Data File : FG007422.D
Signal(s) : FID1A.ch
Acq On : 04 Dec 2020 17:42
Operator : DD\AJ
Sample : L4593-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BARNUM-ST-TP-1

Manual Integrations
APPROVED

Ankita
12/7/2020 12:17:15 PM

Integration File: autoint1.e
Quant Time: Dec 04 21:20:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120220.M
Quant Title :
QLast Update : Thu Dec 03 08:50:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.732	452968	3.533 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120420\
Data File : FG007422.D
Signal(s) : FID1A.ch
Acq On : 04 Dec 2020 17:42
Operator : DD\AJ
Sample : L4593-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
BARNUM-ST-TP-1


Manual Integrations
APPROVED

Ankita
12/7/2020 12:17:15 PM

Integration File: autoint1.e
Quant Time: Dec 04 21:20:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120220.M
Quant Title :
QLast Update : Thu Dec 03 08:50:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

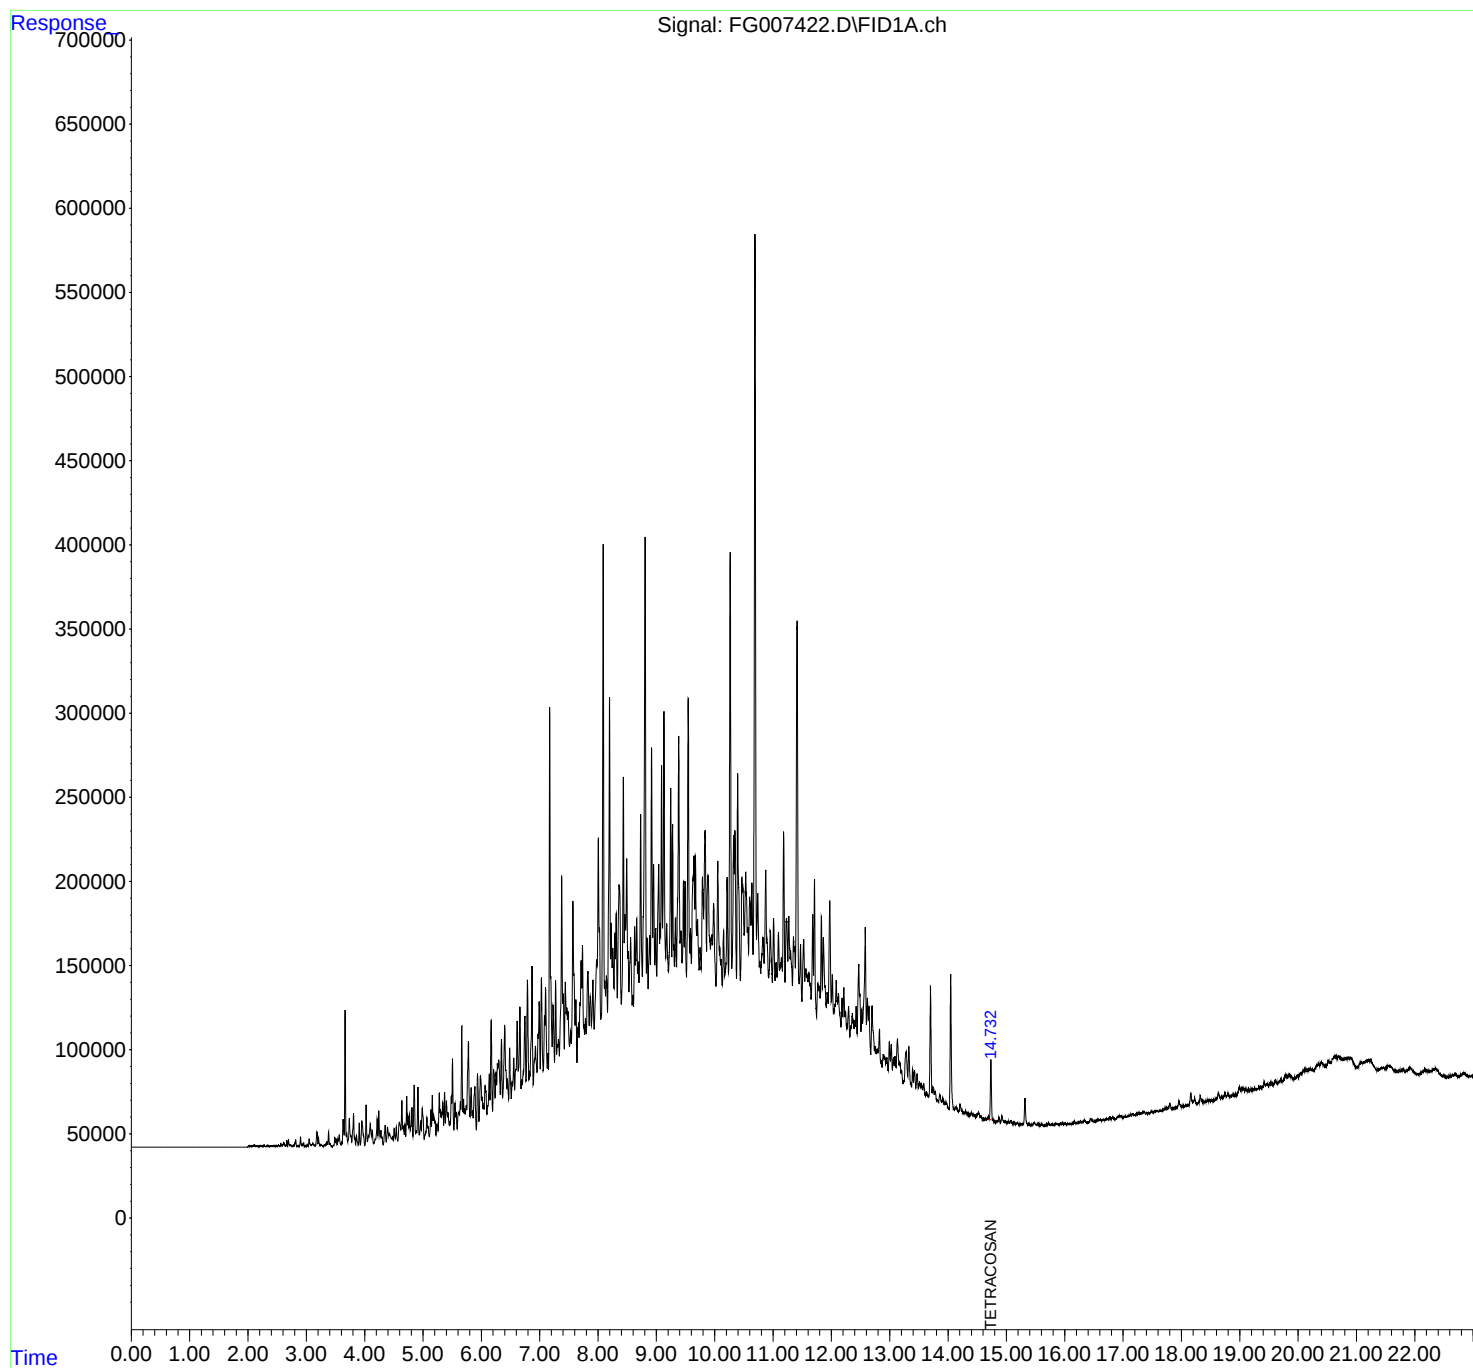

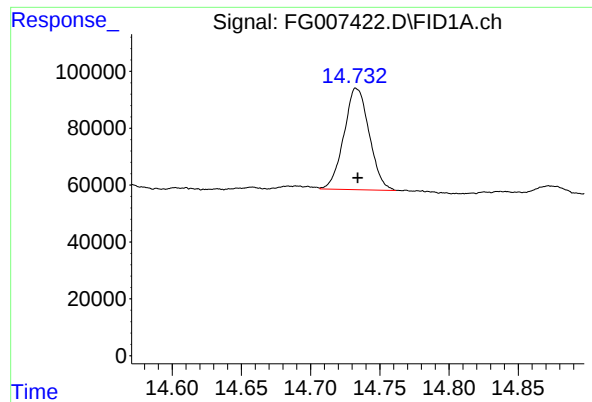

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.732 min
Delta R.T.: -0.002 min
Response: 452968
Conc: 3.53 ug/ml m

Instrument :
FID_G
ClientSampleId :
BARNUM-ST-TP-1

Manual Integrations
APPROVED

Ankita
12/7/2020 12:17:15 PM