

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG120621\  
Data File : FG009165.D  
Signal(s) : FID1A.ch  
Acq On : 06 Dec 2021 11:50  
Operator : AJ\MA  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 07 00:07:22 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG112321.M  
Quant Title :  
QLast Update : Wed Nov 24 00:59:46 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds

|     |                    |        |         |              |
|-----|--------------------|--------|---------|--------------|
| 3)  | N-DODECANE         | 6.465  | 3534316 | 23.876 ug/ml |
| 12) | N-OCTACOSANE       | 16.943 | 2956118 | 25.927 ug/ml |
| 13) | N-TRIACONTANE      | 17.837 | 45202   | 0.418 ug/ml  |
| 14) | N-DOTRIACONTANE    | 18.673 | 54841   | 0.533 ug/ml  |
| 15) | N-TETRATRIACONTANE | 19.459 | 74560   | 0.754 ug/ml  |
| 16) | N-HEXATRIACONTANE  | 20.205 | 35482   | 0.378 ug/ml  |

-----  
(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG120621\  
Data File : FG009165.D  
Signal(s) : FID1A.ch  
Acq On : 06 Dec 2021 11:50  
Operator : AJ\MA  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 07 00:07:22 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG112321.M  
Quant Title :  
QLast Update : Wed Nov 24 00:59:46 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

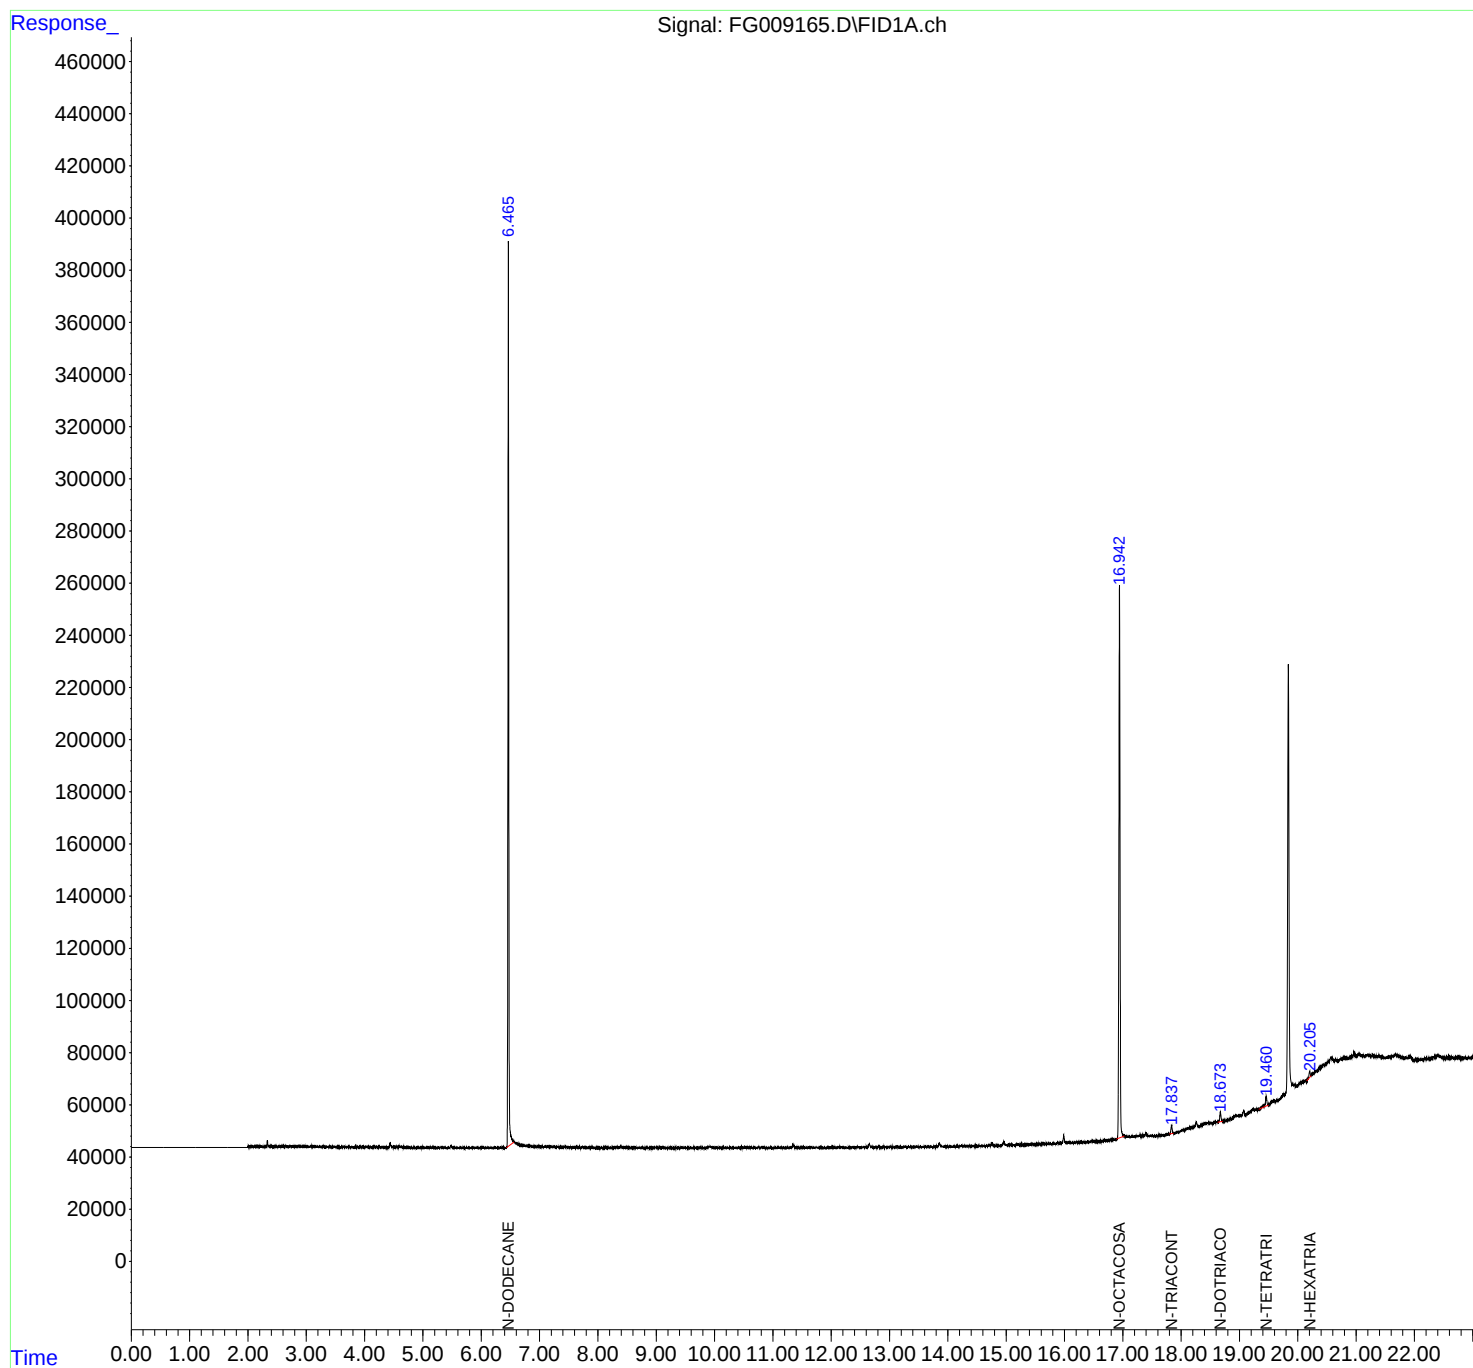


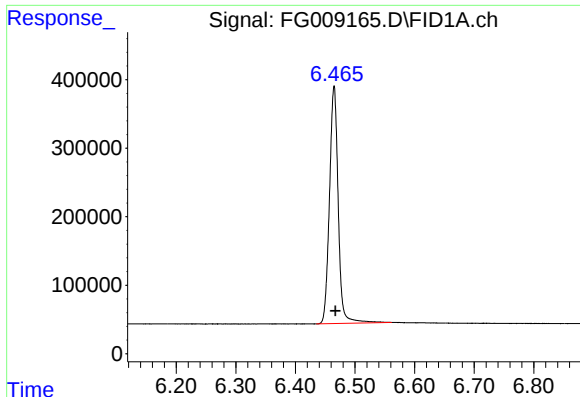

#3 N-DODECANE


R.T.: 6.465 min  
Delta R.T.: -0.002 min  
Response: 3534316  
Conc: 23.88 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

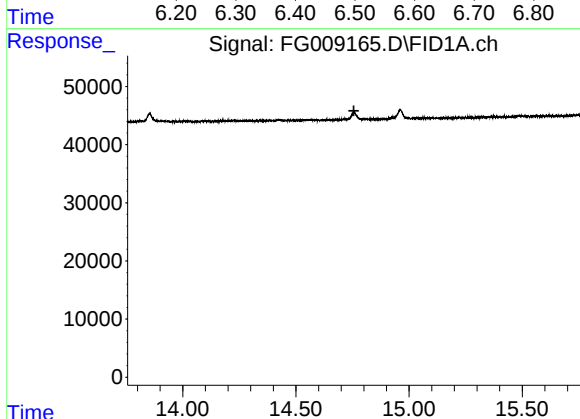


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.756 min  
Response: 0  
Conc: N.D.

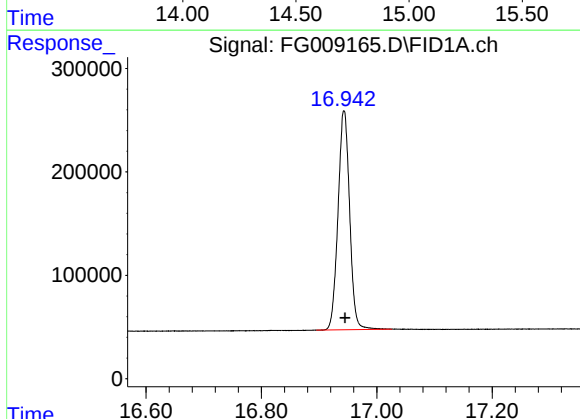


#12 N-OCTACOSANE

R.T.: 16.943 min  
Delta R.T.: -0.001 min  
Response: 2956118  
Conc: 25.93 ug/ml

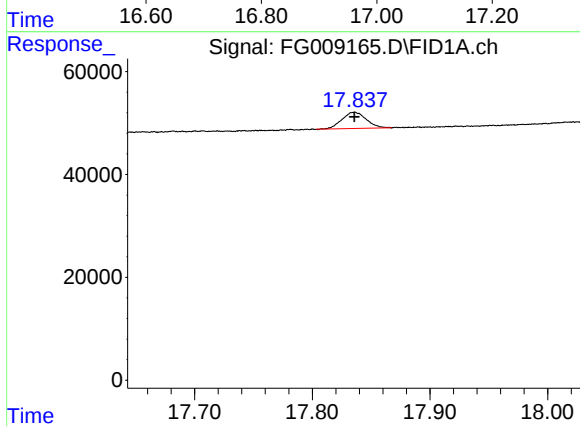

#13 N-TRIACONTANE


R.T.: 17.837 min  
Delta R.T.: 0.000 min  
Response: 45202  
Conc: 0.42 ug/ml

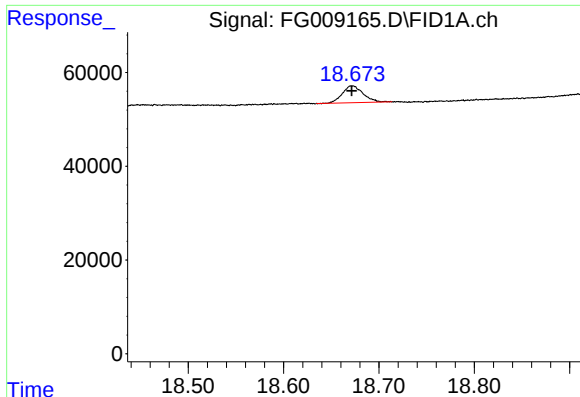

#14 N-DOTRIACONTANE


R.T.: 18.673 min  
Delta R.T.: 0.002 min  
Response: 54841  
Conc: 0.53 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

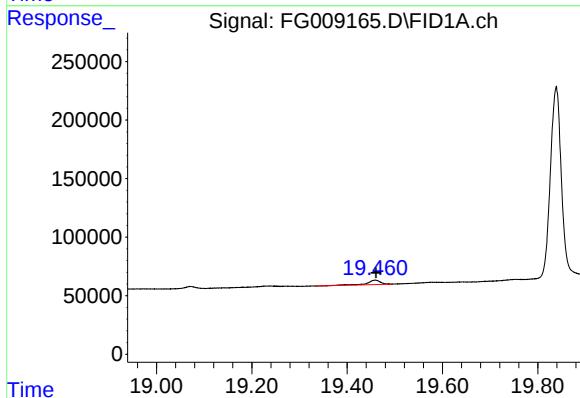

#15 N-TETRATRIACONTANE

R.T.: 19.459 min  
Delta R.T.: 0.000 min  
Response: 74560  
Conc: 0.75 ug/ml

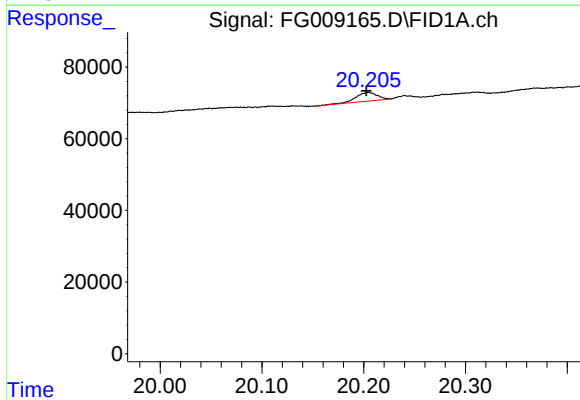

#16 N-HEXATRIACONTANE

R.T.: 20.205 min  
Delta R.T.: 0.002 min  
Response: 35482  
Conc: 0.38 ug/ml