

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120623\
Data File : FG013242.D
Signal(s) : FID1A.ch
Acq On : 06 Dec 2023 13:50
Operator : YP\AJ
Sample : PB157588BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 07 00:06:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120423.M
Quant Title :
QLast Update : Mon Dec 04 11:42:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.080	1833328	17.078 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.985	47613	0.445 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120623\
Data File : FG013242.D
Signal(s) : FID1A.ch
Acq On : 06 Dec 2023 13:50
Operator : YP\AJ
Sample : PB157588BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 07 00:06:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120423.M
Quant Title :
QLast Update : Mon Dec 04 11:42:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

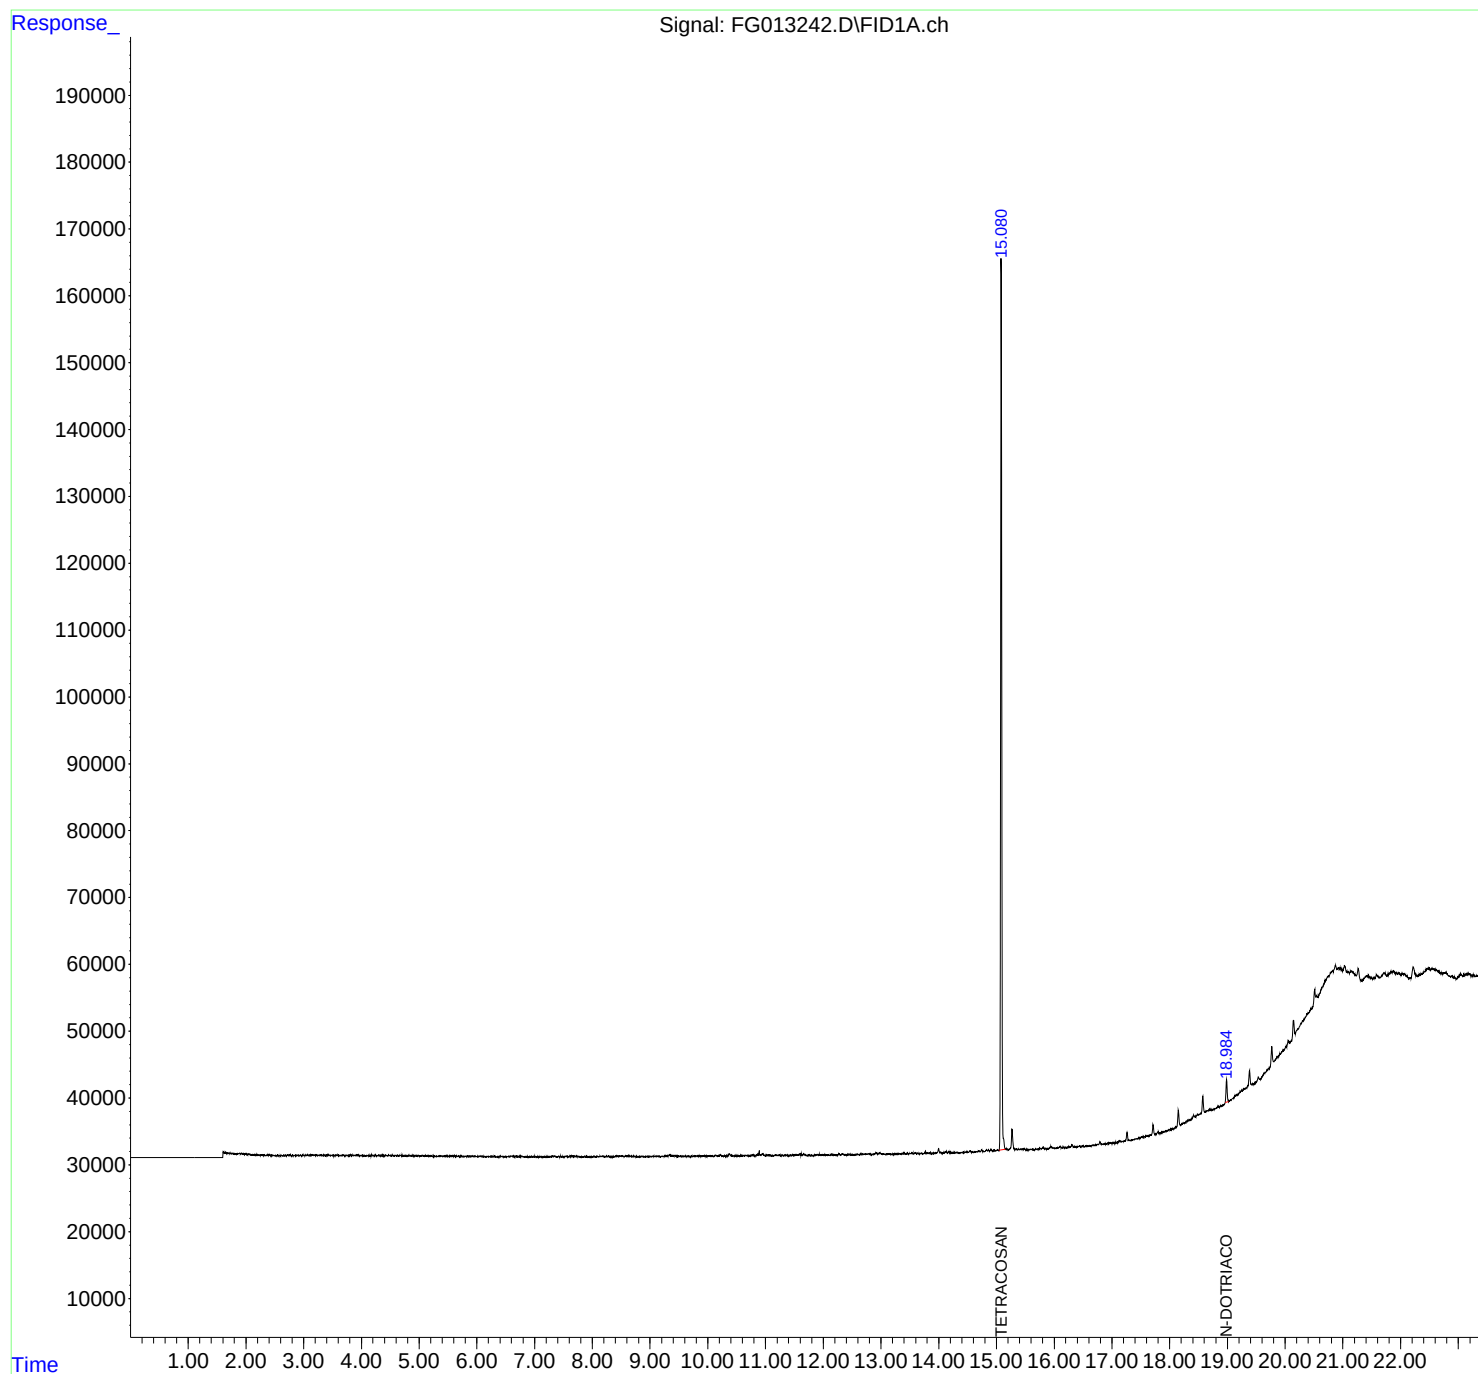


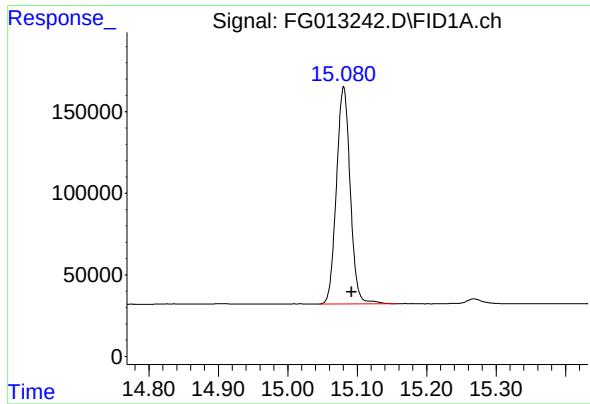

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.080 min
Delta R.T.: -0.012 min
Response: 1833328
Conc: 17.08 ug/ml

Instrument :
FID_G
ClientSampleId :

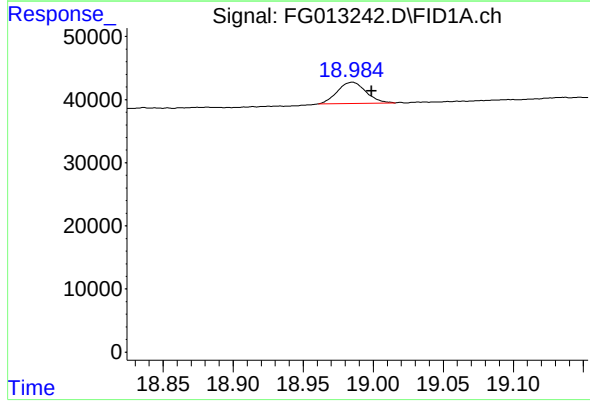

#14 N-DOTRIACONTANE

R.T.: 18.985 min
Delta R.T.: -0.014 min
Response: 47613
Conc: 0.45 ug/ml