

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120718\
 Data File : FG003207.D
 Signal(s) : FID1A.ch
 Acq On : 07 Dec 2018 20:16
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 08 00:48:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
 Quant Title :
 QLast Update : Thu Nov 29 04:54:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.714	5132915	47.100 ug/ml
Target Compounds			
2) N-DECANE	4.416	6530160	55.882 ug/ml
3) N-DODECANE	6.443	6540483	54.985 ug/ml
4) N-TETRADECANE	8.243	6499296	53.494 ug/ml
5) N-HEXADECANE	9.848	6429828	51.850 ug/ml
6) N-OCTADECANE	11.294	6309617	50.194 ug/ml
7) N-EICOSANE	12.608	6110939	48.697 ug/ml
8) N-DOCOSANE	13.811	5927680	47.400 ug/ml
10) N-TETRACOSANE	14.919	5781087	46.512 ug/ml
11) N-HEXACOSANE	15.946	5690544	45.800 ug/ml
12) N-OCTACOSANE	16.901	5675664	45.543 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120718\
Data File : FG003207.D
Signal(s) : FID1A.ch
Acq On : 07 Dec 2018 20:16
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 08 00:48:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112818.M
Quant Title :
QLast Update : Thu Nov 29 04:54:55 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

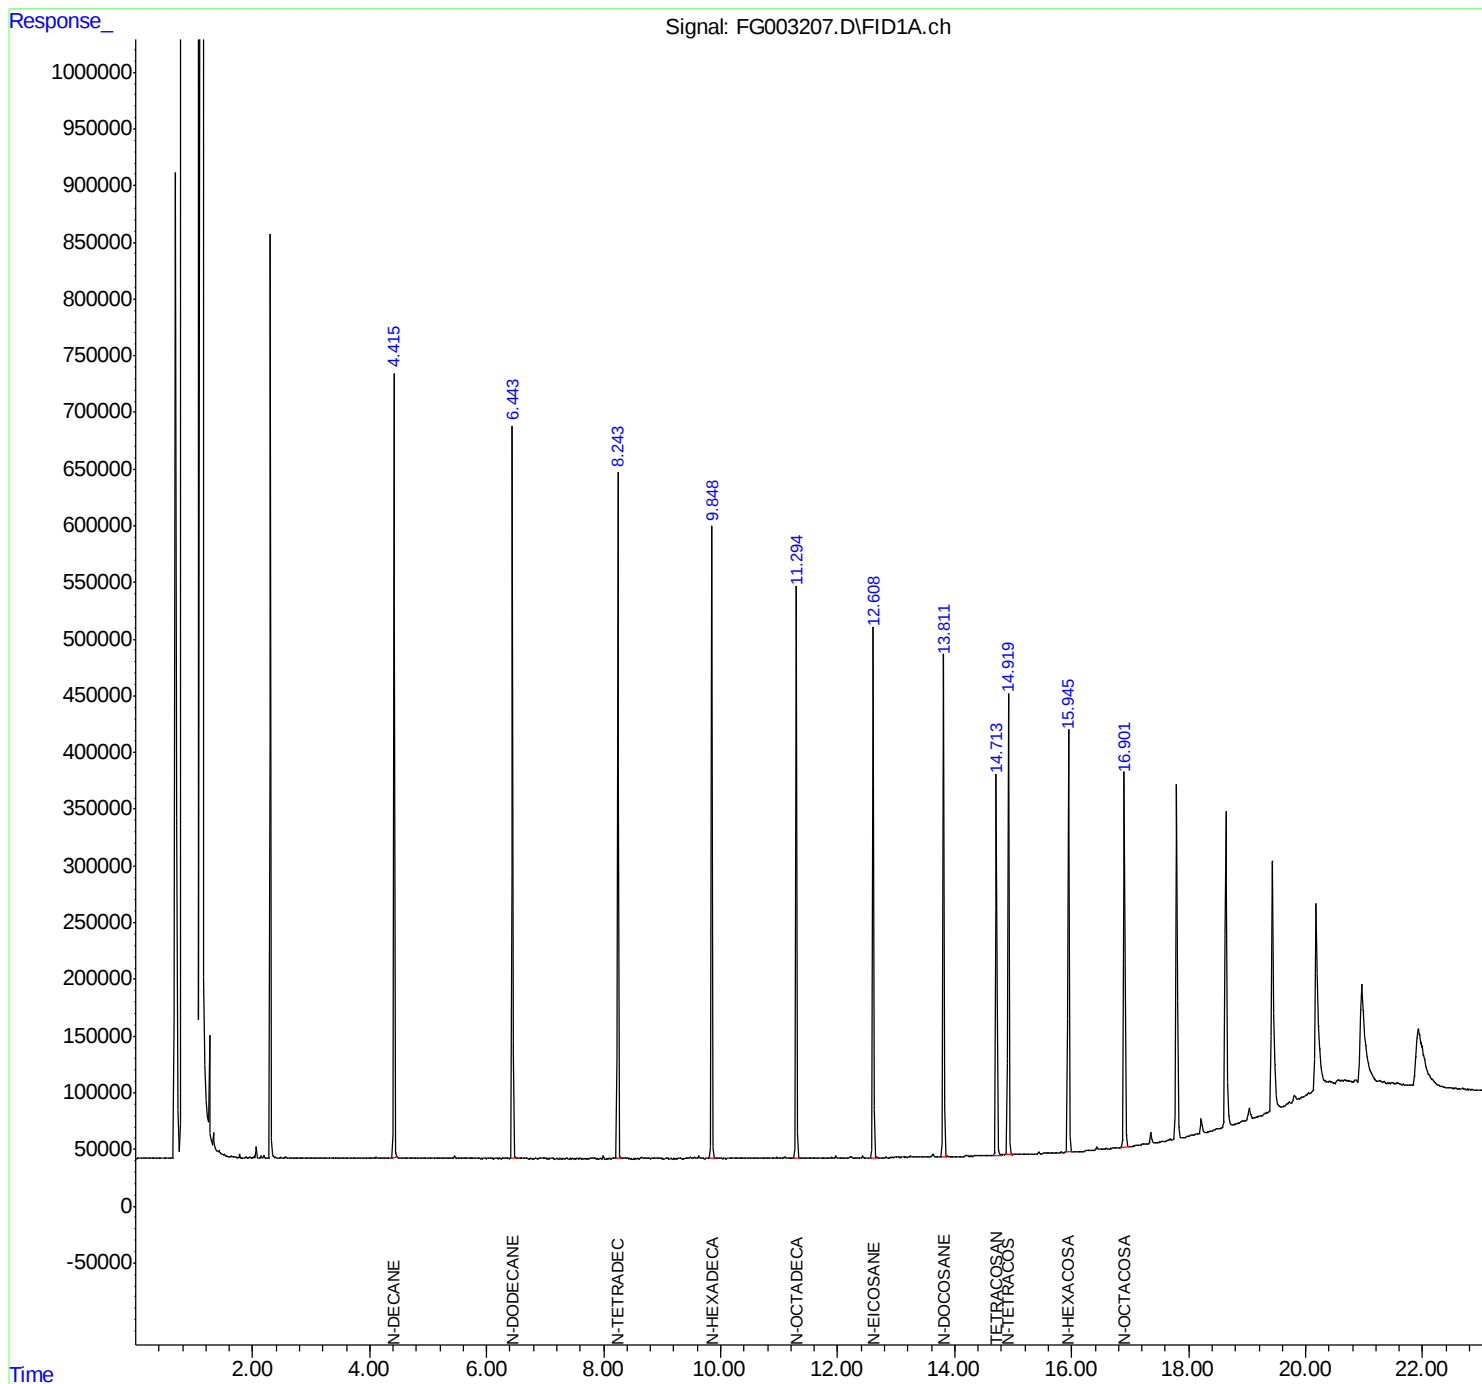

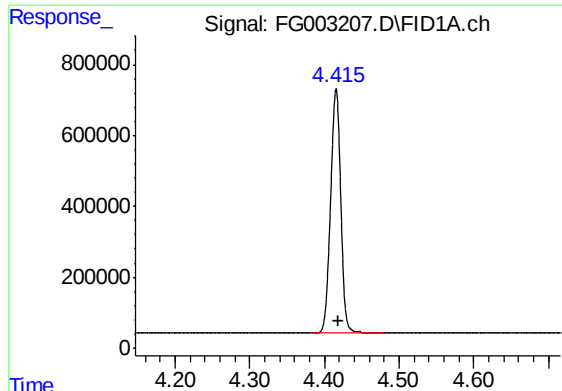


#2 N-DECANE

R.T.: 4.416 min
Delta R.T.: -0.004 min
Response: 6530160
Conc: 55.88 ug/ml

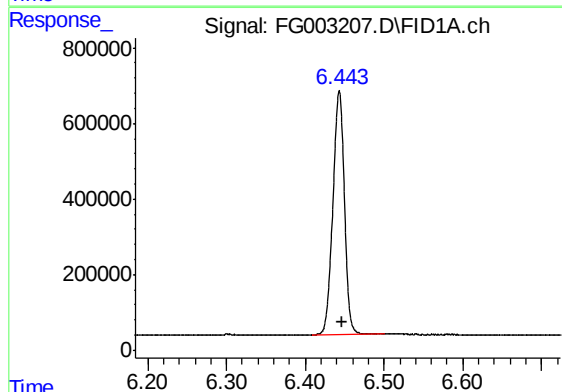


#3 N-DODECANE

R.T.: 6.443 min
Delta R.T.: -0.003 min
Response: 6540483
Conc: 54.98 ug/ml

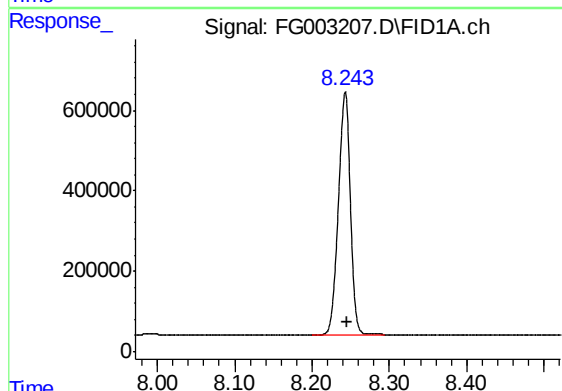


#4 N-TETRADECANE

R.T.: 8.243 min
Delta R.T.: -0.003 min
Response: 6499296
Conc: 53.49 ug/ml

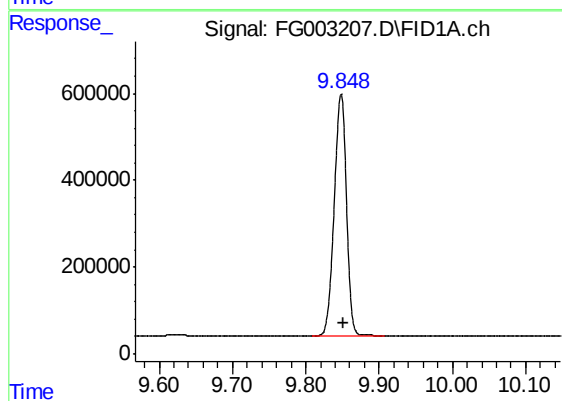


#5 N-HEXADECANE

R.T.: 9.848 min
Delta R.T.: -0.003 min
Response: 6429828
Conc: 51.85 ug/ml

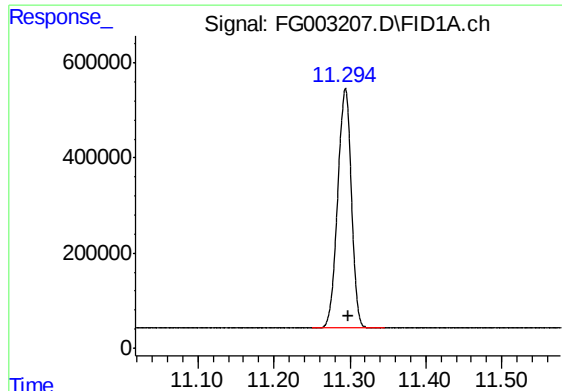


#6 N-OCTADECANE

R.T.: 11.294 min
Delta R.T.: -0.003 min
Response: 6309617
Conc: 50.19 ug/ml

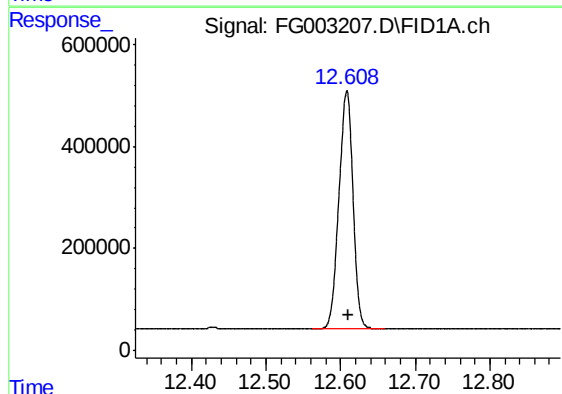


#7 N-EICOSANE

R.T.: 12.608 min
Delta R.T.: -0.003 min
Response: 6110939
Conc: 48.70 ug/ml

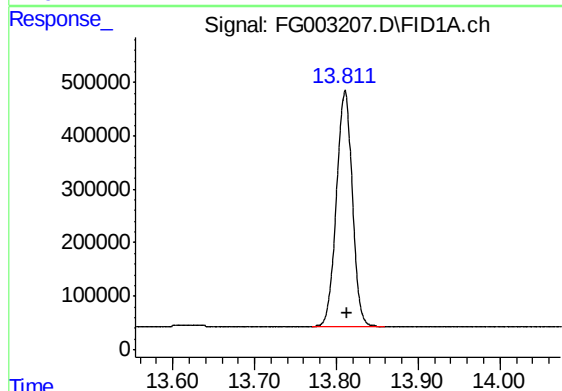


#8 N-DOCOSANE

R.T.: 13.811 min
Delta R.T.: -0.003 min
Response: 5927680
Conc: 47.40 ug/ml

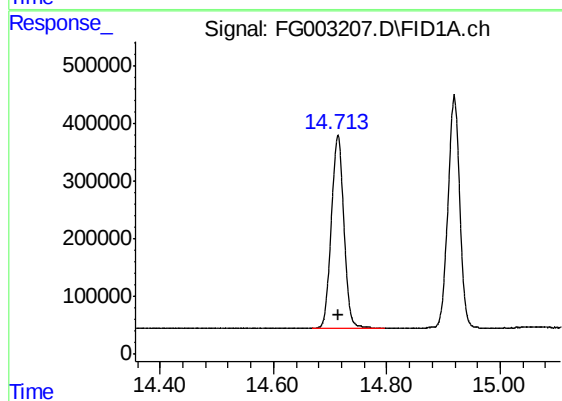


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.714 min
Delta R.T.: -0.001 min
Response: 5132915
Conc: 47.10 ug/ml

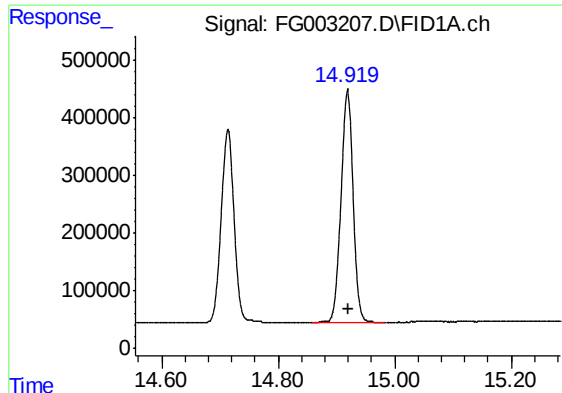


#10 N-TETRACOSANE

R.T.: 14.919 min
Delta R.T.: -0.002 min
Response: 5781087
Conc: 46.51 ug/ml

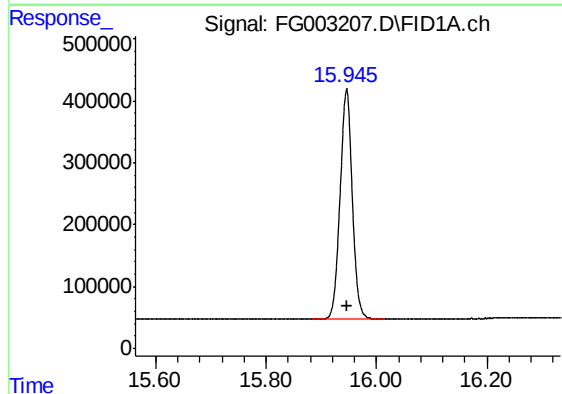

#11 N-HEXACOSANE

R.T.: 15.946 min
Delta R.T.: 0.000 min
Response: 5690544
Conc: 45.80 ug/ml

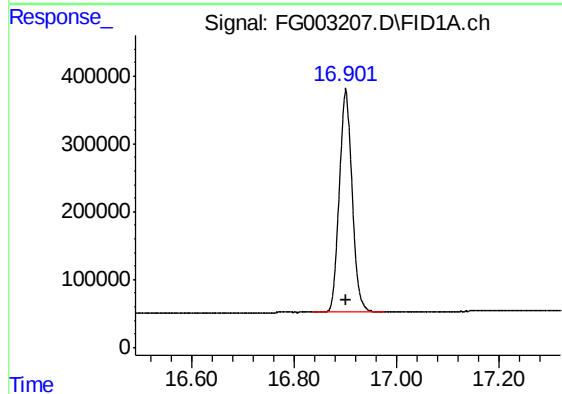

#12 N-OCTACOSANE

R.T.: 16.901 min
Delta R.T.: 0.000 min
Response: 5675664
Conc: 45.54 ug/ml