

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG120720\  
Data File : FG007428.D  
Signal(s) : FID1A.ch  
Acq On : 07 Dec 2020 11:52  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Dec 07 14:18:09 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG120220.M  
Quant Title :  
QLast Update : Thu Dec 03 08:50:10 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.461  | 4293236  | 28.492 ug/ml |
| 12) N-OCTACOSANE            | 16.916 | 3730232  | 26.866 ug/ml |
| -----                       |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG120720\  
Data File : FG007428.D  
Signal(s) : FID1A.ch  
Acq On : 07 Dec 2020 11:52  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Dec 07 14:18:09 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG120220.M  
Quant Title :  
QLast Update : Thu Dec 03 08:50:10 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

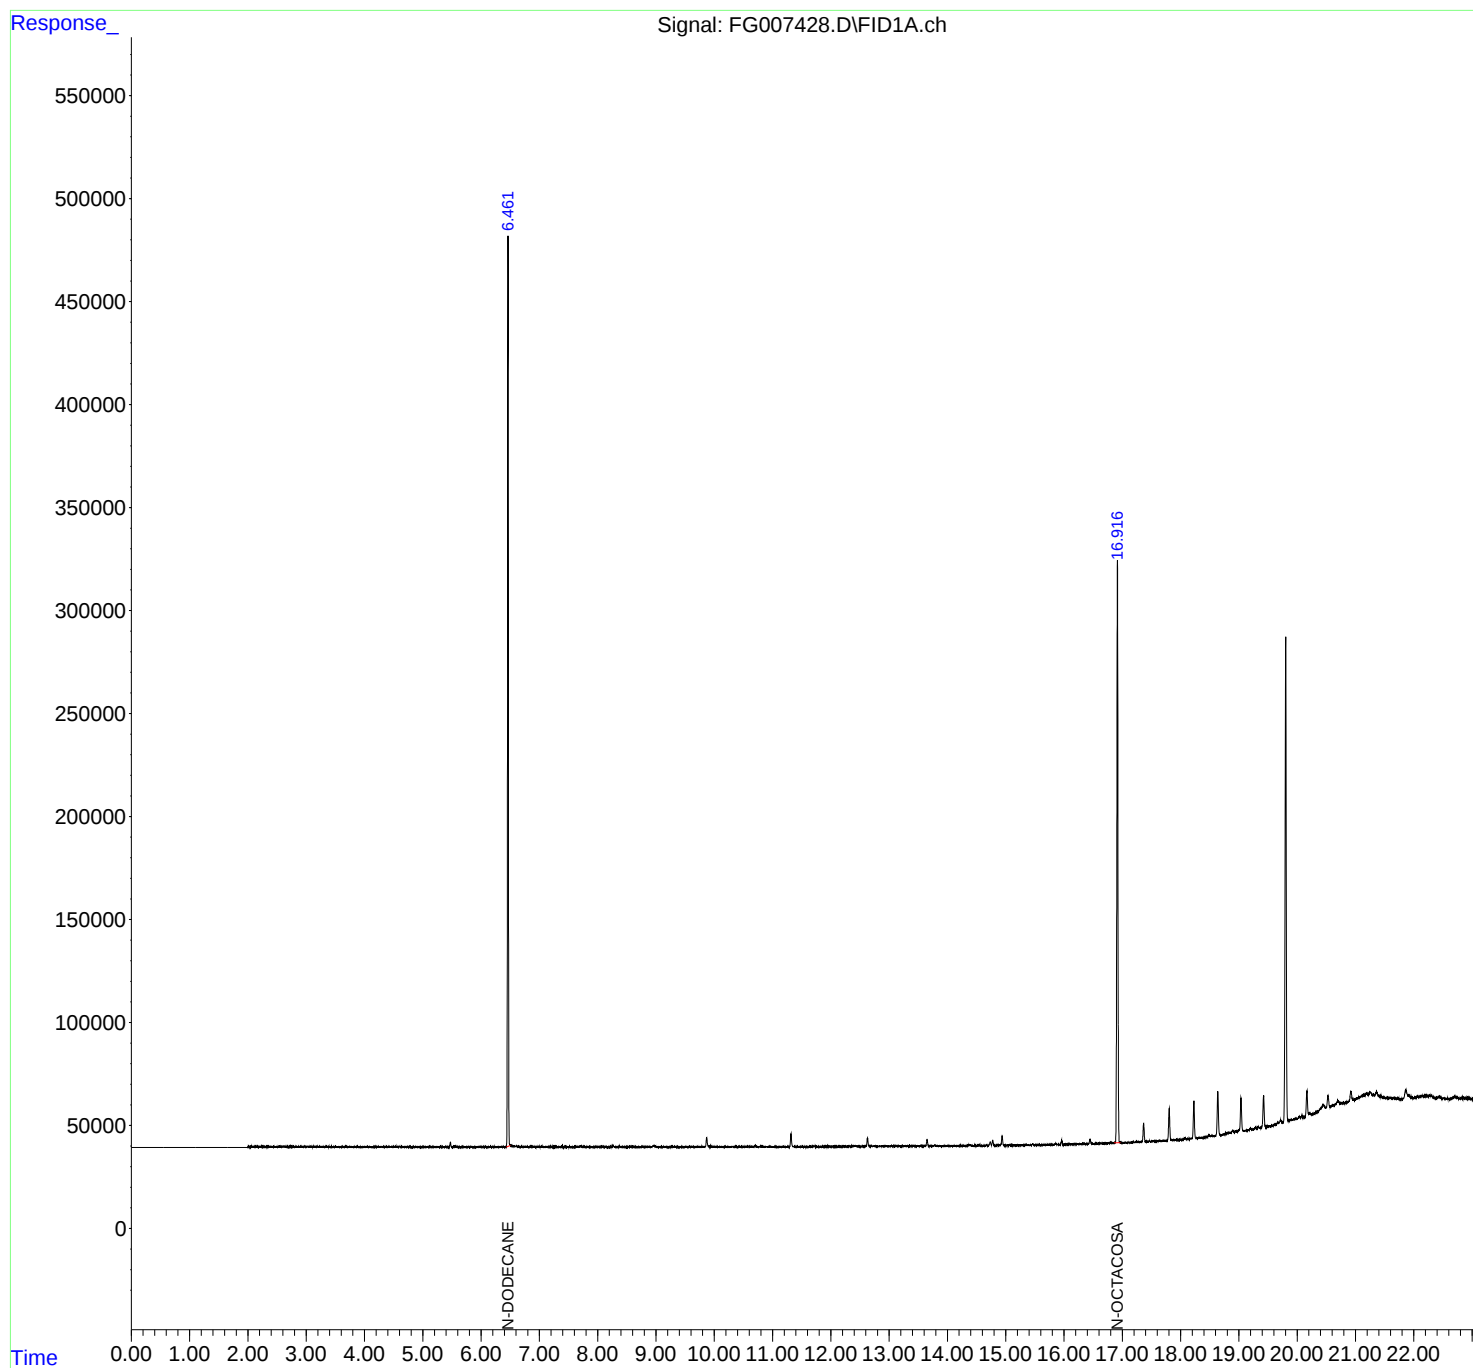

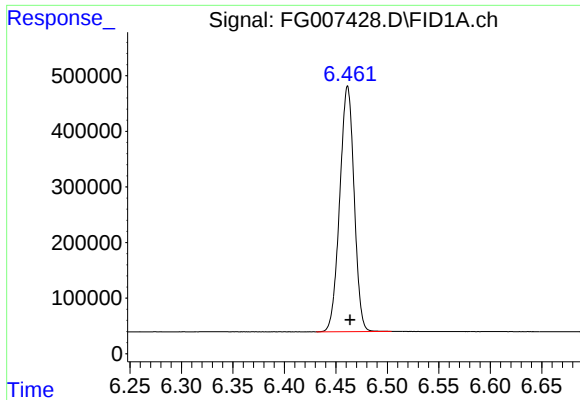


#3 N-DODECANE

R.T.: 6.461 min  
Delta R.T.: -0.002 min  
Response: 4293236  
Conc: 28.49 ug/ml

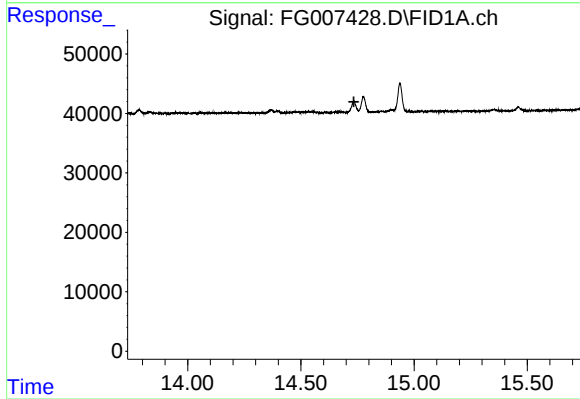

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.734 min  
Response: 0  
Conc: N.D.

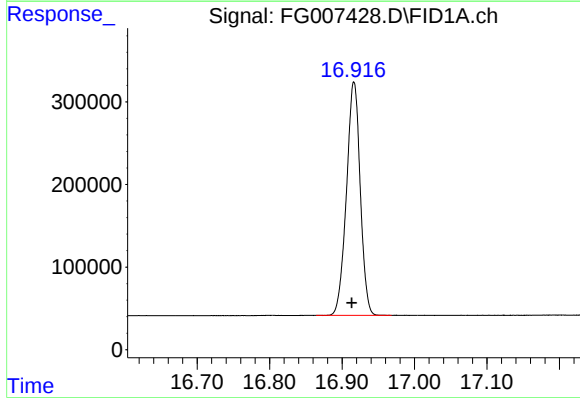

#12 N-OCTACOSANE

R.T.: 16.916 min  
Delta R.T.: 0.003 min  
Response: 3730232  
Conc: 26.87 ug/ml