

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120722\
Data File : FG011193.D
Signal(s) : FID1A.ch
Acq On : 07 Dec 2022 13:03
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 08 01:33:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120522.M
Quant Title :
QLast Update : Tue Dec 06 04:53:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.766	2765021	20.289 ug/ml
12) N-OCTACOSANE	17.257	2532959	20.538 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120722\
Data File : FG011193.D
Signal(s) : FID1A.ch
Acq On : 07 Dec 2022 13:03
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 08 01:33:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120522.M
Quant Title :
QLast Update : Tue Dec 06 04:53:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

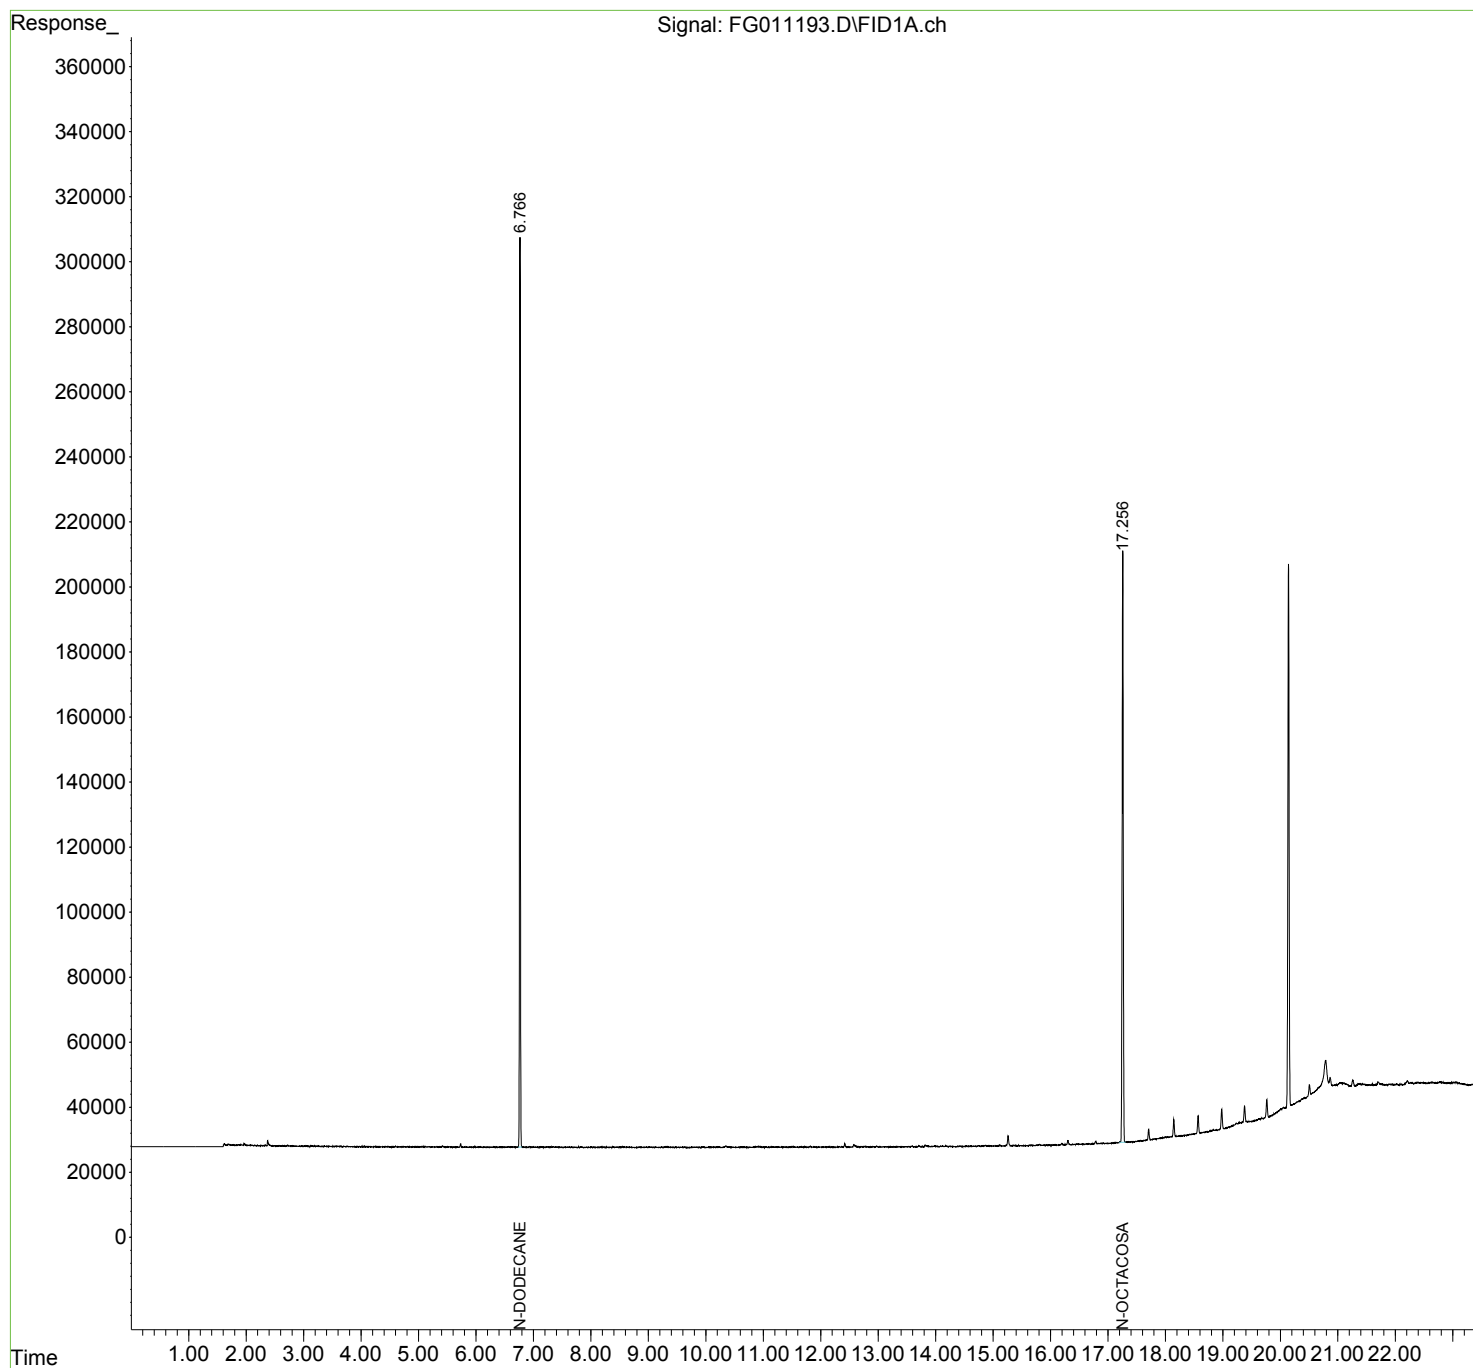


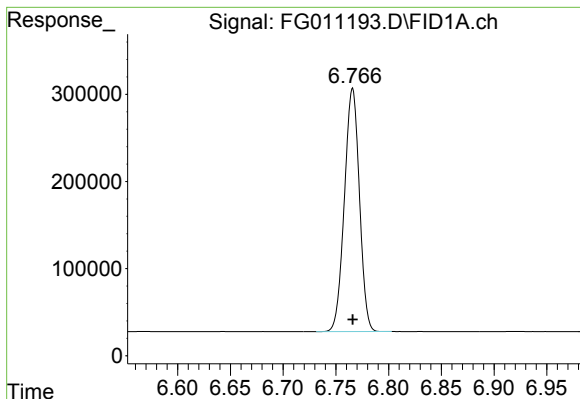

#3 N-DODECANE


R.T.: 6.766 min
 Delta R.T.: 0.000 min
 Response: 2765021
 Conc: 20.29 ug/ml

Instrument :
 FID_G
 ClientSampleId :
 RT MARKER

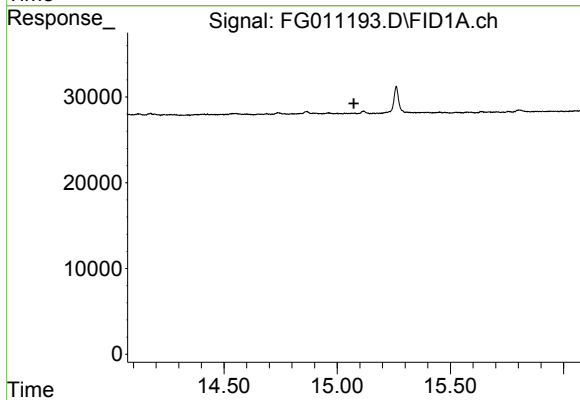

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
 Exp R.T. : 15.074 min
 Response: 0
 Conc: N.D.

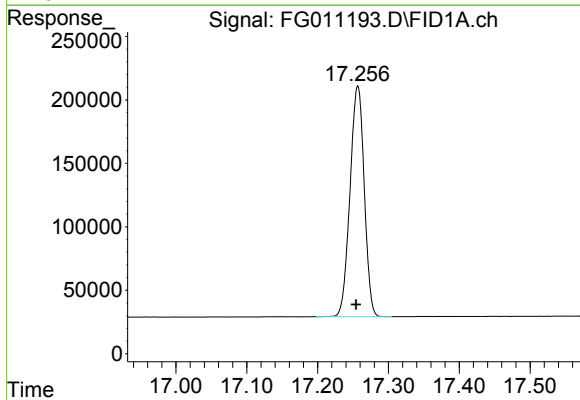

#12 N-OCTACOSANE

R.T.: 17.257 min
 Delta R.T.: 0.003 min
 Response: 2532959
 Conc: 20.54 ug/ml