

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120921\
Data File : FG009186.D
Signal(s) : FID1A.ch
Acq On : 09 Dec 2021 18:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 09 21:37:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	1963866	16.839 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.144f	13151	0.140 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG120921\
Data File : FG009186.D
Signal(s) : FID1A.ch
Acq On : 09 Dec 2021 18:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 09 21:37:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

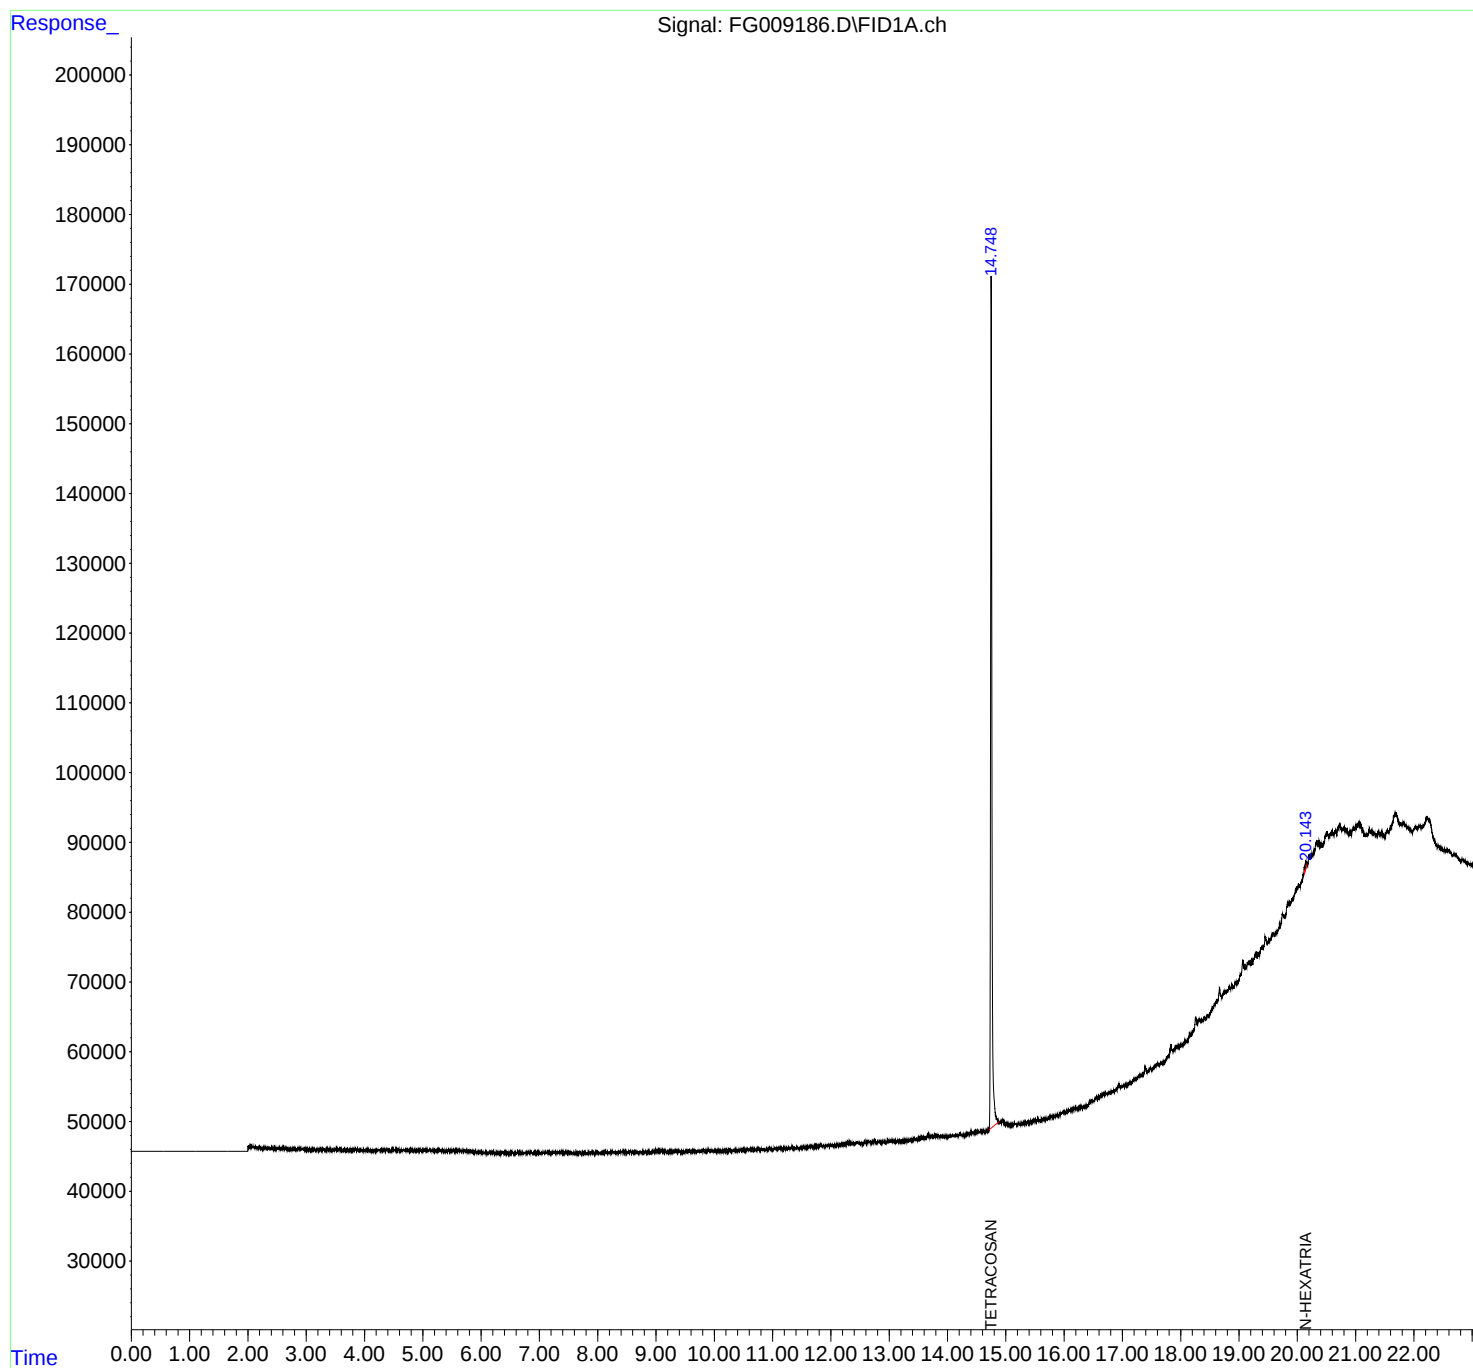


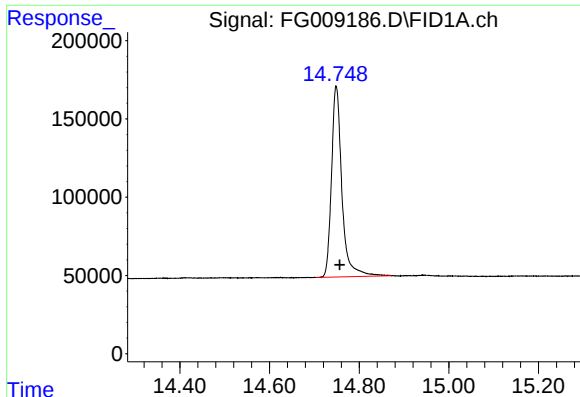

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.749 min
Delta R.T.: -0.008 min
Response: 1963866
Conc: 16.84 ug/ml

Instrument :
FID_G
ClientSampleId :

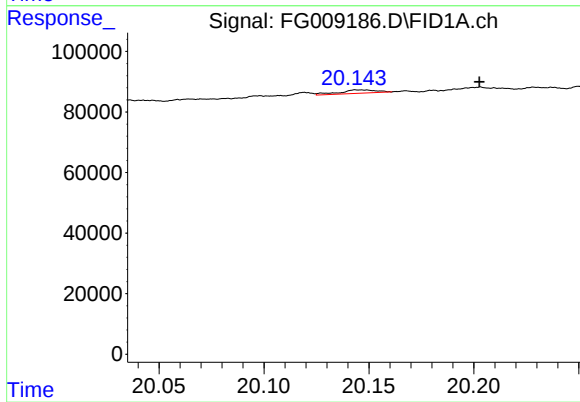

#16 N-HEXATRIACONTANE

R.T.: 20.144 min
Delta R.T.: -0.059 min
Response: 13151
Conc: 0.14 ug/ml